


Real Time PCR

=

Quantitative PCR (qPCR)


(RT-qPCR = reverse-transcription – quantitative PCR)

Michał Koper, IGiB UW

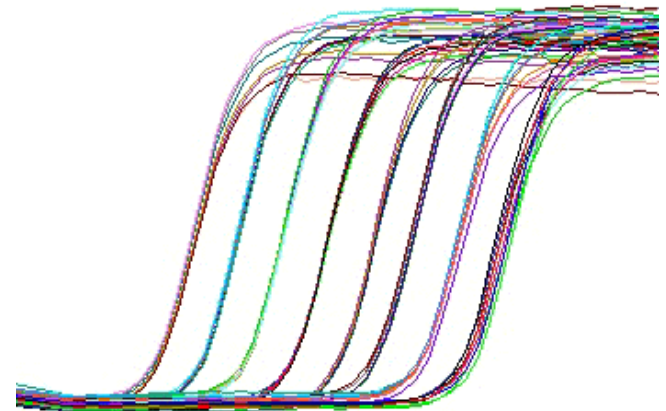


Pioneering work on qPCR (also known as kinetic PCR)

- **Higuchi R., Dollinger G., Walsh P.S., Griffith R. (1992). Simultaneous amplification and detection of specific DNA sequences. Biotechnology 10:413-7.**
- **Higuchi R., Fockler C., Dollinger G., Watson R. (1993). Kinetic PCR analysis: real-time monitoring of DNA amplification reactions. Biotechnology 11:1026 -30.**



Applications of qPCR:

- **Gene expression analysis (RT-qPCR)**
- **Detection of nucleic acids of pathogens:** detecting the presence and determining the concentration of viruses and bacteria in serum
- **Genotyping: SNP or HRM analyses**
- **Detection of GMOs in feed and food**




qPCR is based on detection of PCR product increment over time

- Method is based on the determination of the DNA concentration for each reaction cycle, using **fluorescence**
- Fluorescent dyes binds dsDNA directly (**nonspecific detection**) or dyes are coupled with hybridization probes (**specific detection** - targeted to a selected strand of the **amplicon** under study)

amplicon = PCR product, PCR fragment

- Requires **excitation system**: halogen lamp, LED system or laser
- Requires **detection system**: separate CCD elements, CCD array or photomultiplier circuits



Examples of qPCR cyclers



Roche LightCycler 480




QIAGEN Rotor-Gene Q





**BioRad
CFX96/
CFX384**




Appliedbiosystems 7900HT




qPCR cycler scheme

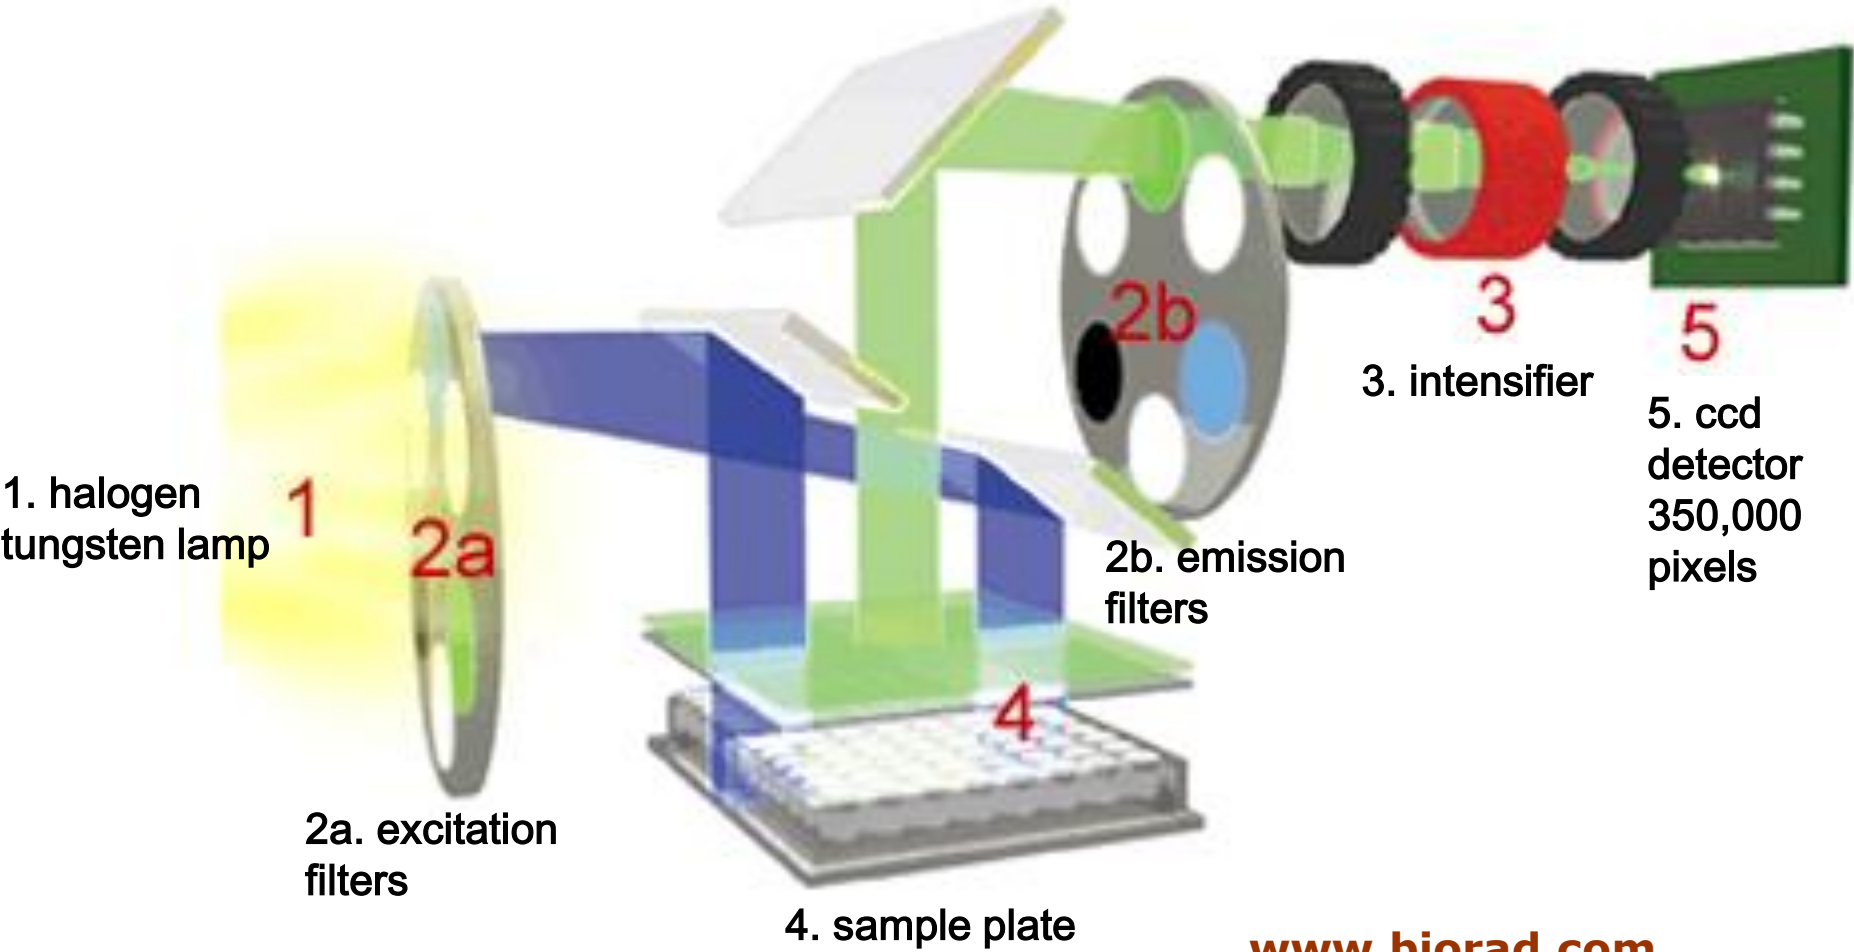

How to detect DNA products in qPCR?




DNA-binding dyes: SYBR Green

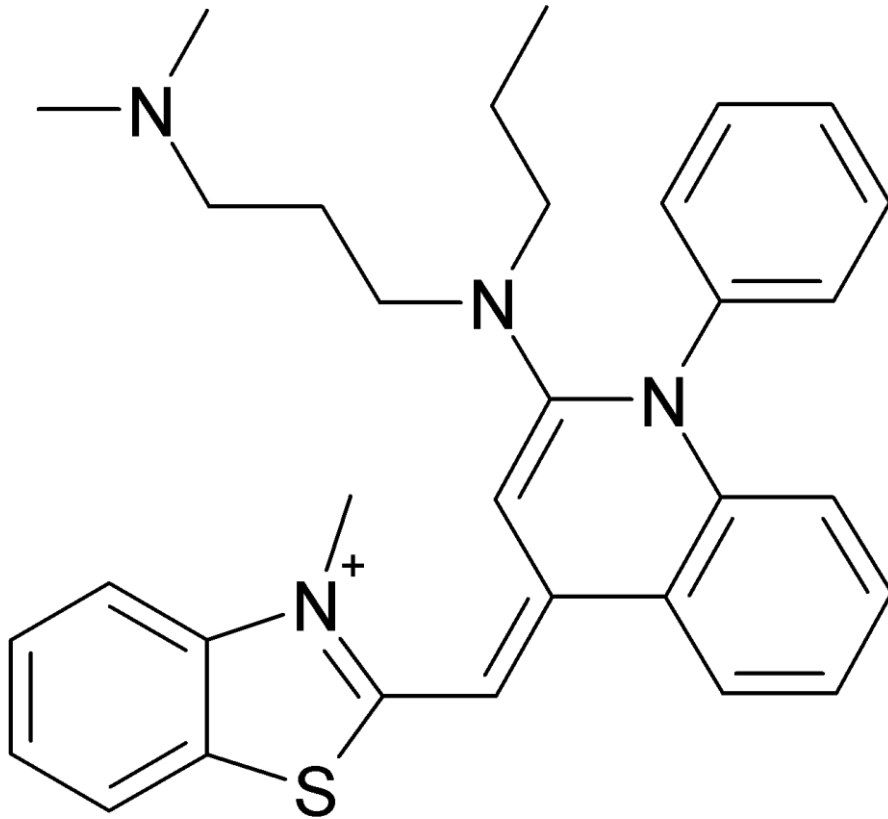


SYBR Green I, Wikipedia


- Belongs to **cyanine dyes** (containing heterocyclic rings with **-C=** bonds)
- Binds **dsDNA**, weakly **ssDNA**
- Excited by blue light ($\lambda_{\text{max}} = 488 \text{ nm}$)
- Emits green light ($\lambda_{\text{max}} = 522 \text{ nm}$)



SYBR Green

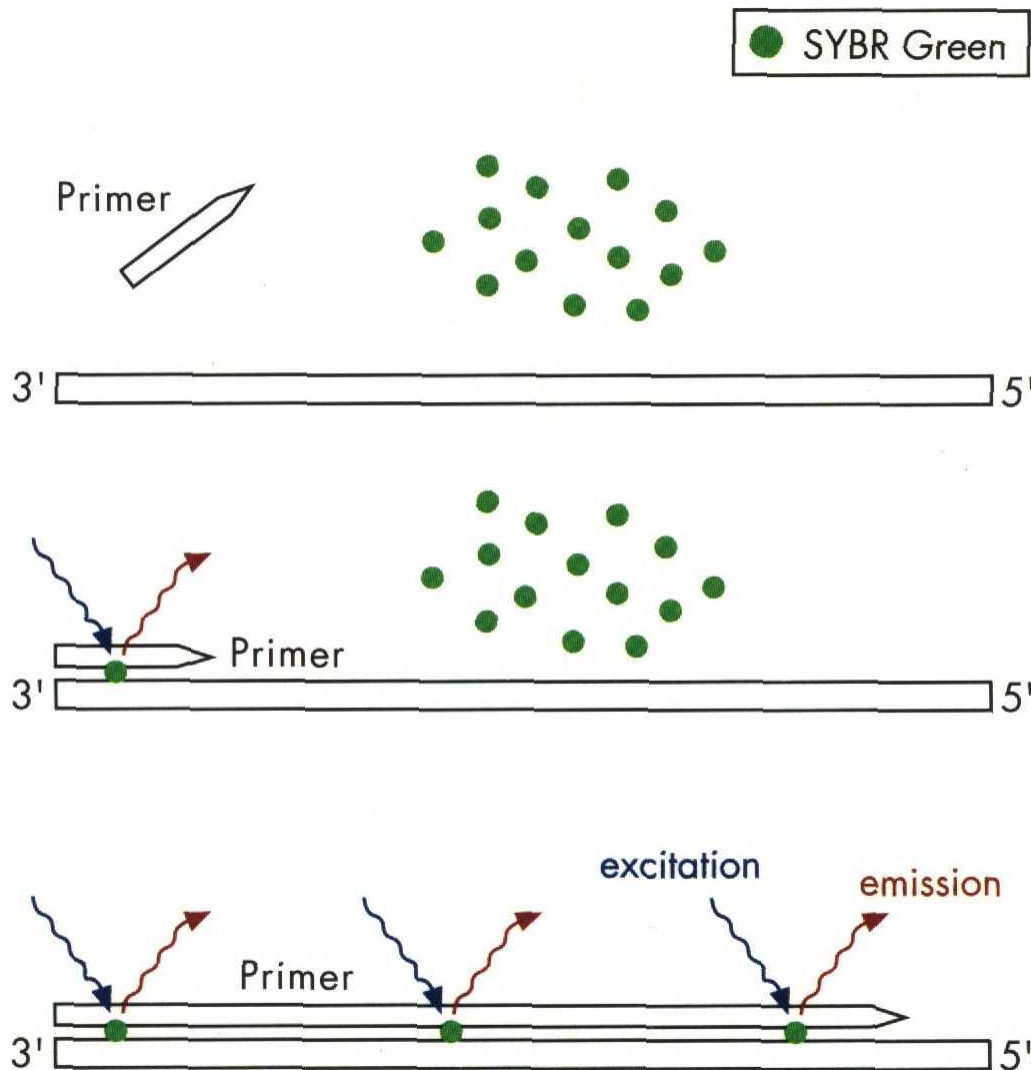


- Detects any **dsDNA**
- Detection at the **ELONGATION** stage
- Primers cannot form **PRIMER-DIMERS**
- Product size preferably in the range of **100-200 bp**
- The size of the detected products for different genes must be **VERY CLOSE**
- Enables the analysis of **MELTING CURVES**
- **THE CHEAPEST** method




qPCR primers design

- Length of the amplicon preferably less than **150 bp**
- Avoid **sequence complementarity** within a **primer** or between **primers** = "primer dimer"
- Avoid unpaired bases
- Preferably **G or C at the 3' end**, never T
- Length of primers **18-30 nt**
- GC content **40-60%**
- **$T_m = (A+T) \times 2^\circ\text{C} + (G+C) \times 4^\circ\text{C}$**
- **Use at least 2 programs and compare results!!!**
Different software = different algorithms (not always...)!






Hybridization probes




TaqMan – hydrolysis probes

DNA Pol Exo !!!+

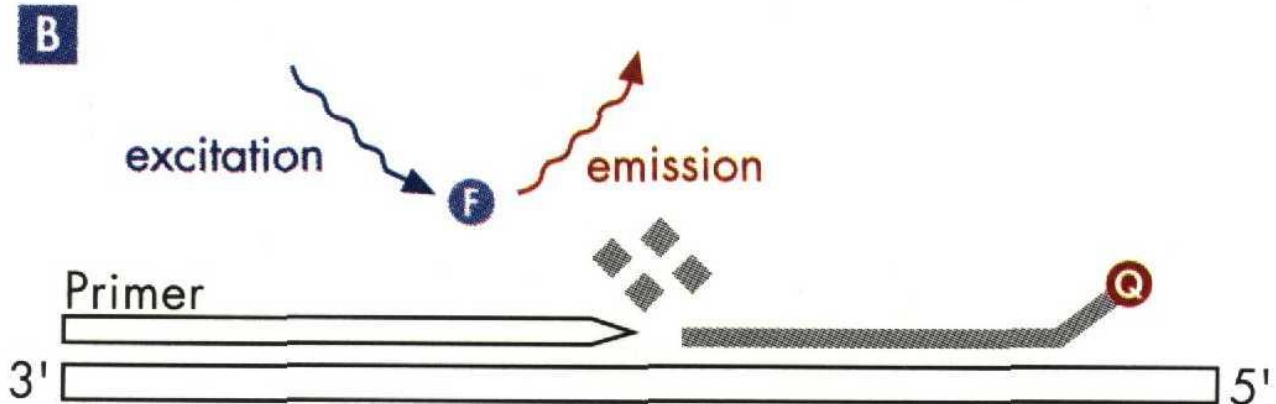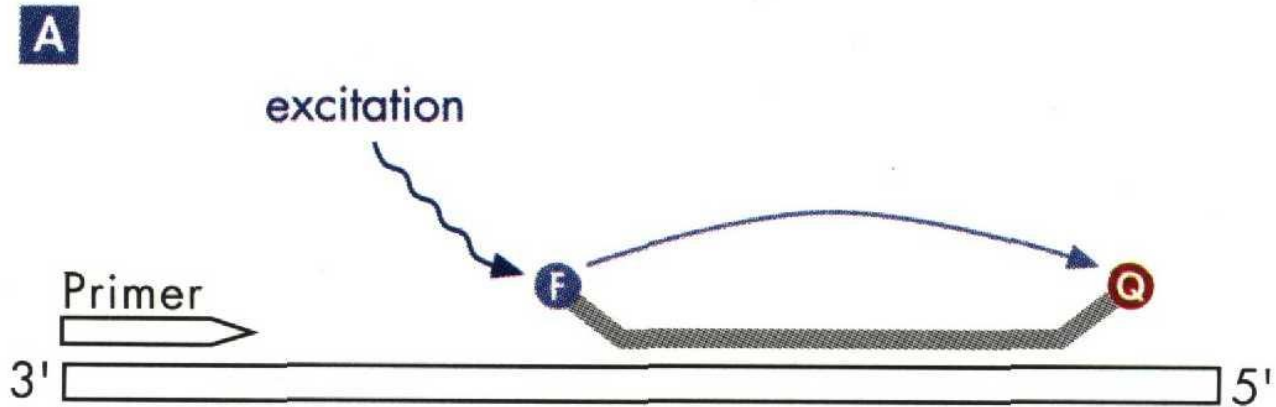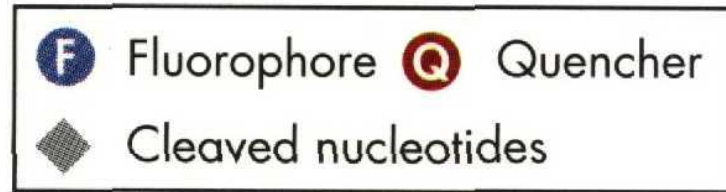


ABI, Roche (UPL)





TaqMan probe – design principles

- Short amplicons: **70-150 bp**
- **$T_m = 68-70^\circ\text{C}$**
- GC content **30-60%**
- Never **G at the 5' end** (G is natural quencher)
- Probe length **max. 30 nt**
- Avoid strings of identical bases
- Avoid secondary structures
- Avoid complementarity with primers
- Choose a strand with a higher C content




Multiplex qPCR

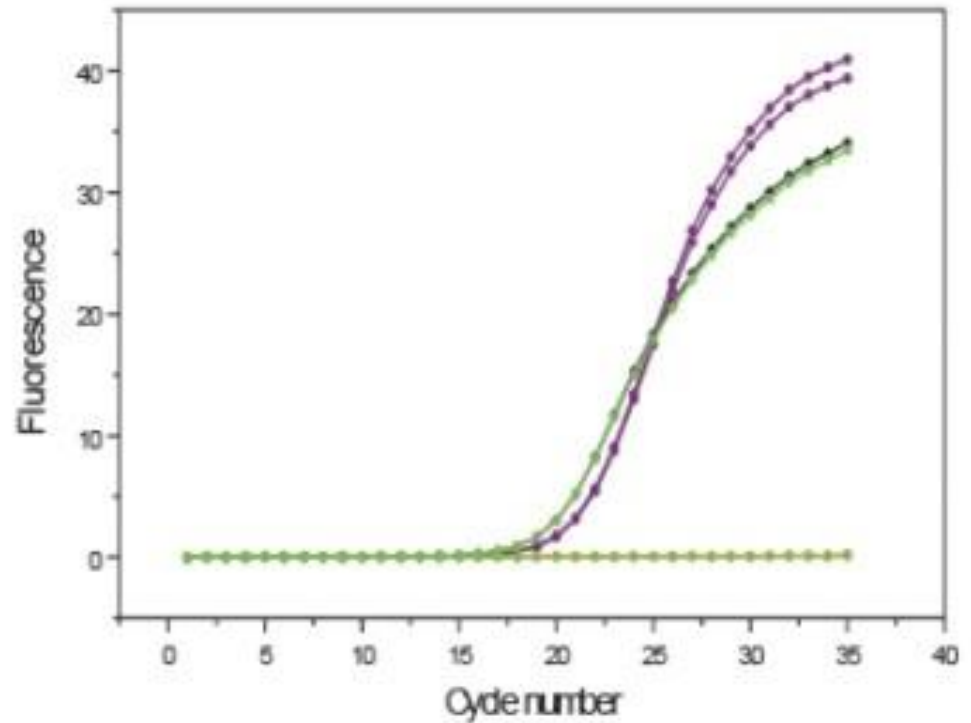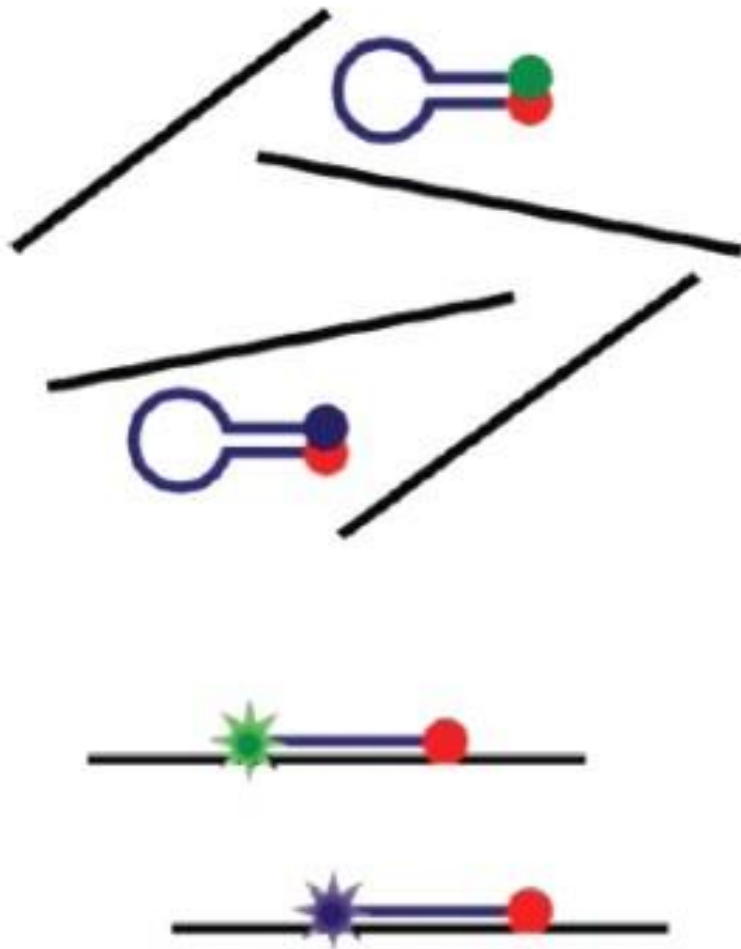


Different detection formats and different dyes allow detection of 2 or more products in a single reaction


(not possible with SYBR Green!!!)



Determination of the RNA levels




Classic northern-blot technique

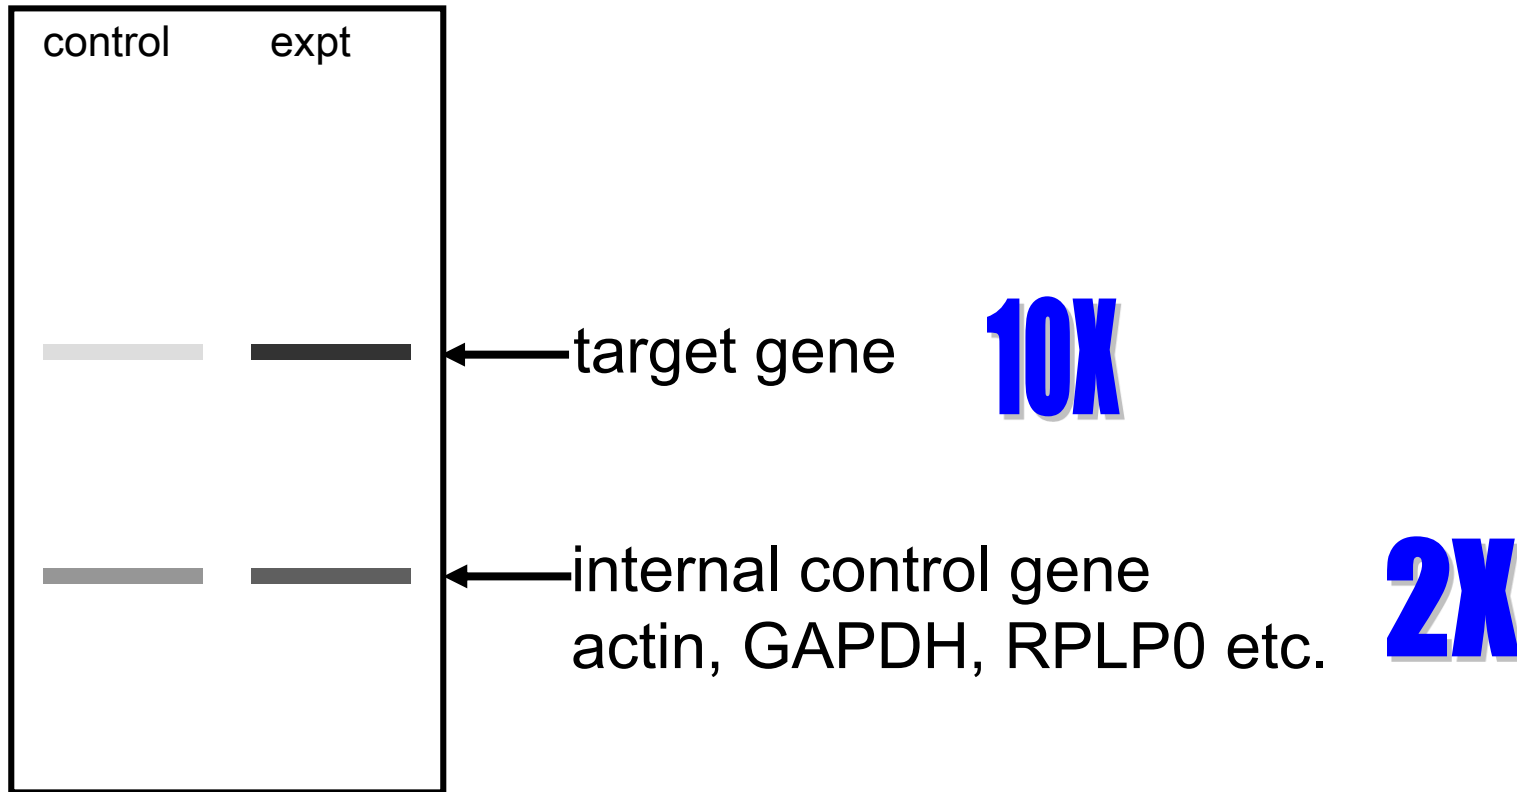


Corrected fold increase = $10/2 = 5$

Ratio target gene in experimental/control = $\frac{\text{fold change in target gene}}{\text{fold change in reference gene}}$




Theoretical basis of qPCR




| CYCLE NUMBER | AMOUNT OF DNA |
|--------------|---------------|
| 0 | 1 |
| 1 | 2 |
| 2 | 4 |
| 3 | 8 |
| 4 | 16 |
| 5 | 32 |
| 6 | 64 |
| 7 | 128 |
| 8 | 256 |
| 9 | 512 |
| 10 | 1,024 |
| 11 | 2,048 |
| 12 | 4,096 |
| 13 | 8,192 |
| 14 | 16,384 |
| 15 | 32,768 |
| 16 | 65,536 |
| 17 | 131,072 |
| 18 | 262,144 |
| 19 | 524,288 |
| 20 | 1,048,576 |
| 21 | 2,097,152 |
| 22 | 4,194,304 |
| 23 | 8,388,608 |
| 24 | 16,777,216 |
| 25 | 33,554,432 |
| 26 | 67,108,864 |
| 27 | 134,217,728 |
| 28 | 268,435,456 |
| 29 | 536,870,912 |
| 30 | 1,073,741,824 |
| 31 | 1,400,000,000 |
| 32 | 1,500,000,000 |
| 33 | 1,550,000,000 |
| 34 | 1,580,000,000 |

Theoretical curve

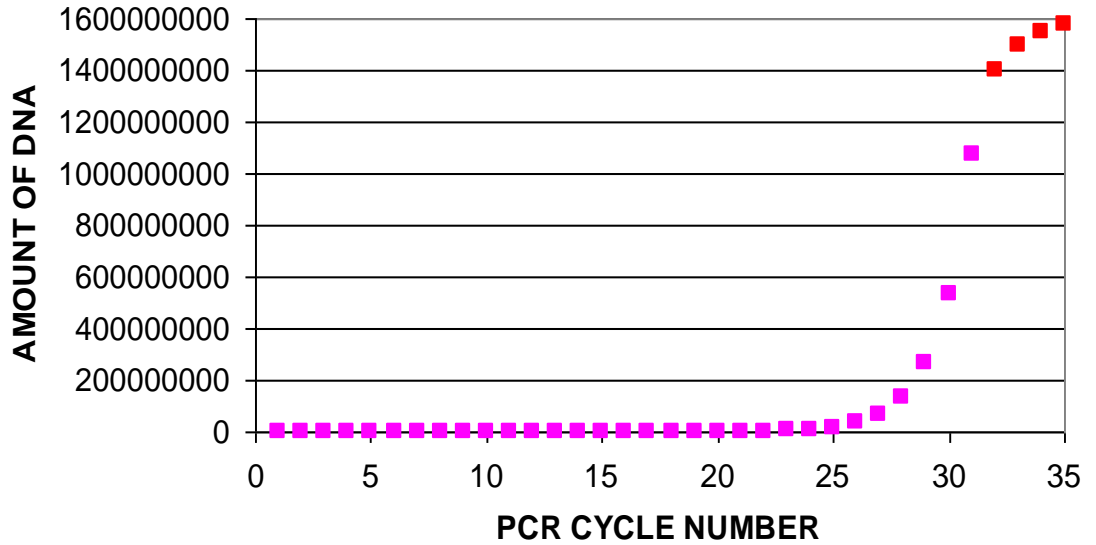


Transformed on a logarithmic scale

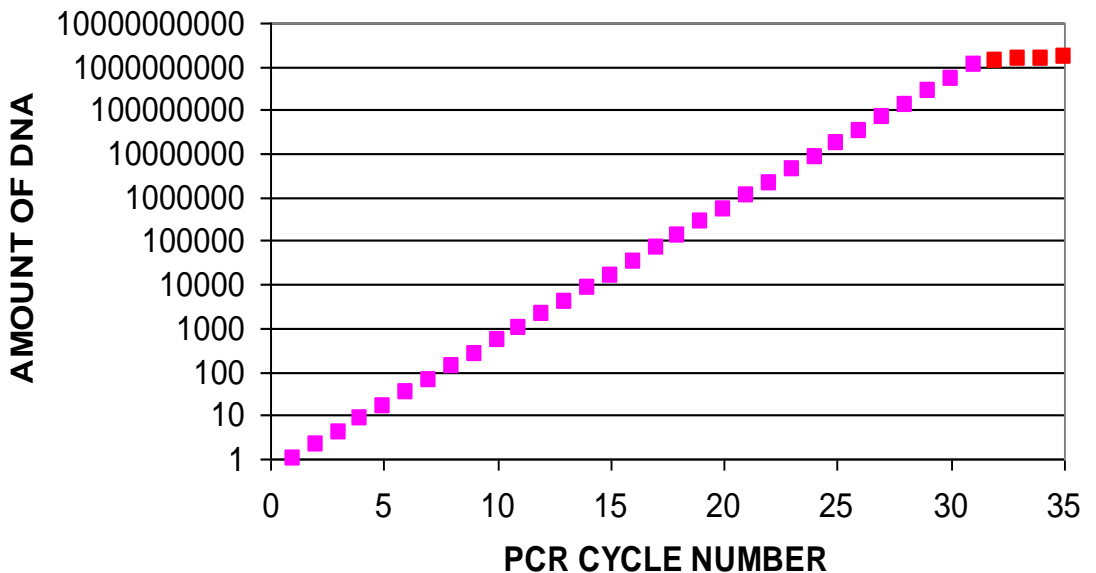



4 phases of the qPCR reaction

- **Phase 1** : fluorescence at background level, reaction occurs exponentially but detection is not possible
- **Phase 2**: exponential growth detectable, fluorescence above background
- **Phase 3**: a "steep" increase in fluorescence allows detection that the reaction is occurring linearly
- **Phase 4 - plateau**: breakdown and saturation of the reaction


M. W. Pfaffl: *Quantification strategies in real-time PCR* in *A-Z of quantitative PCR* (Editor: S.A. Bustin)



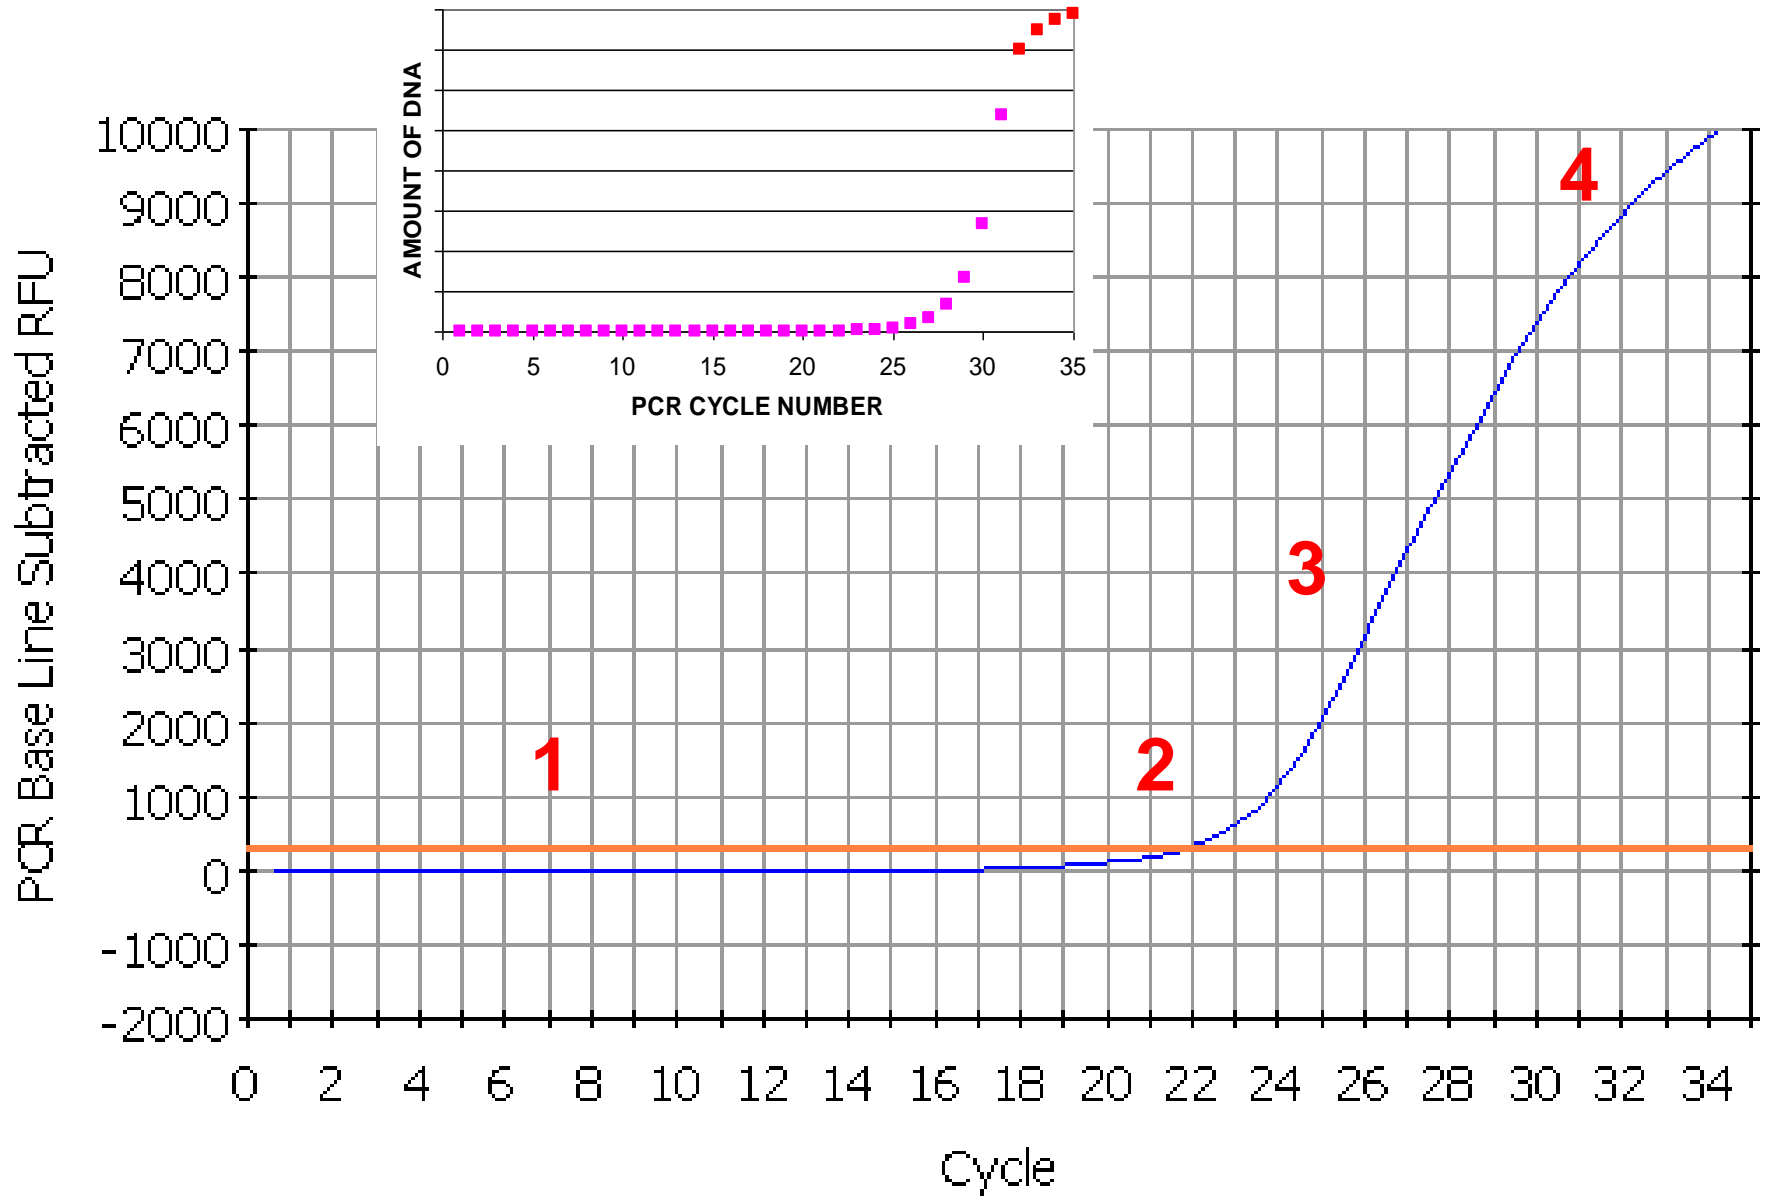


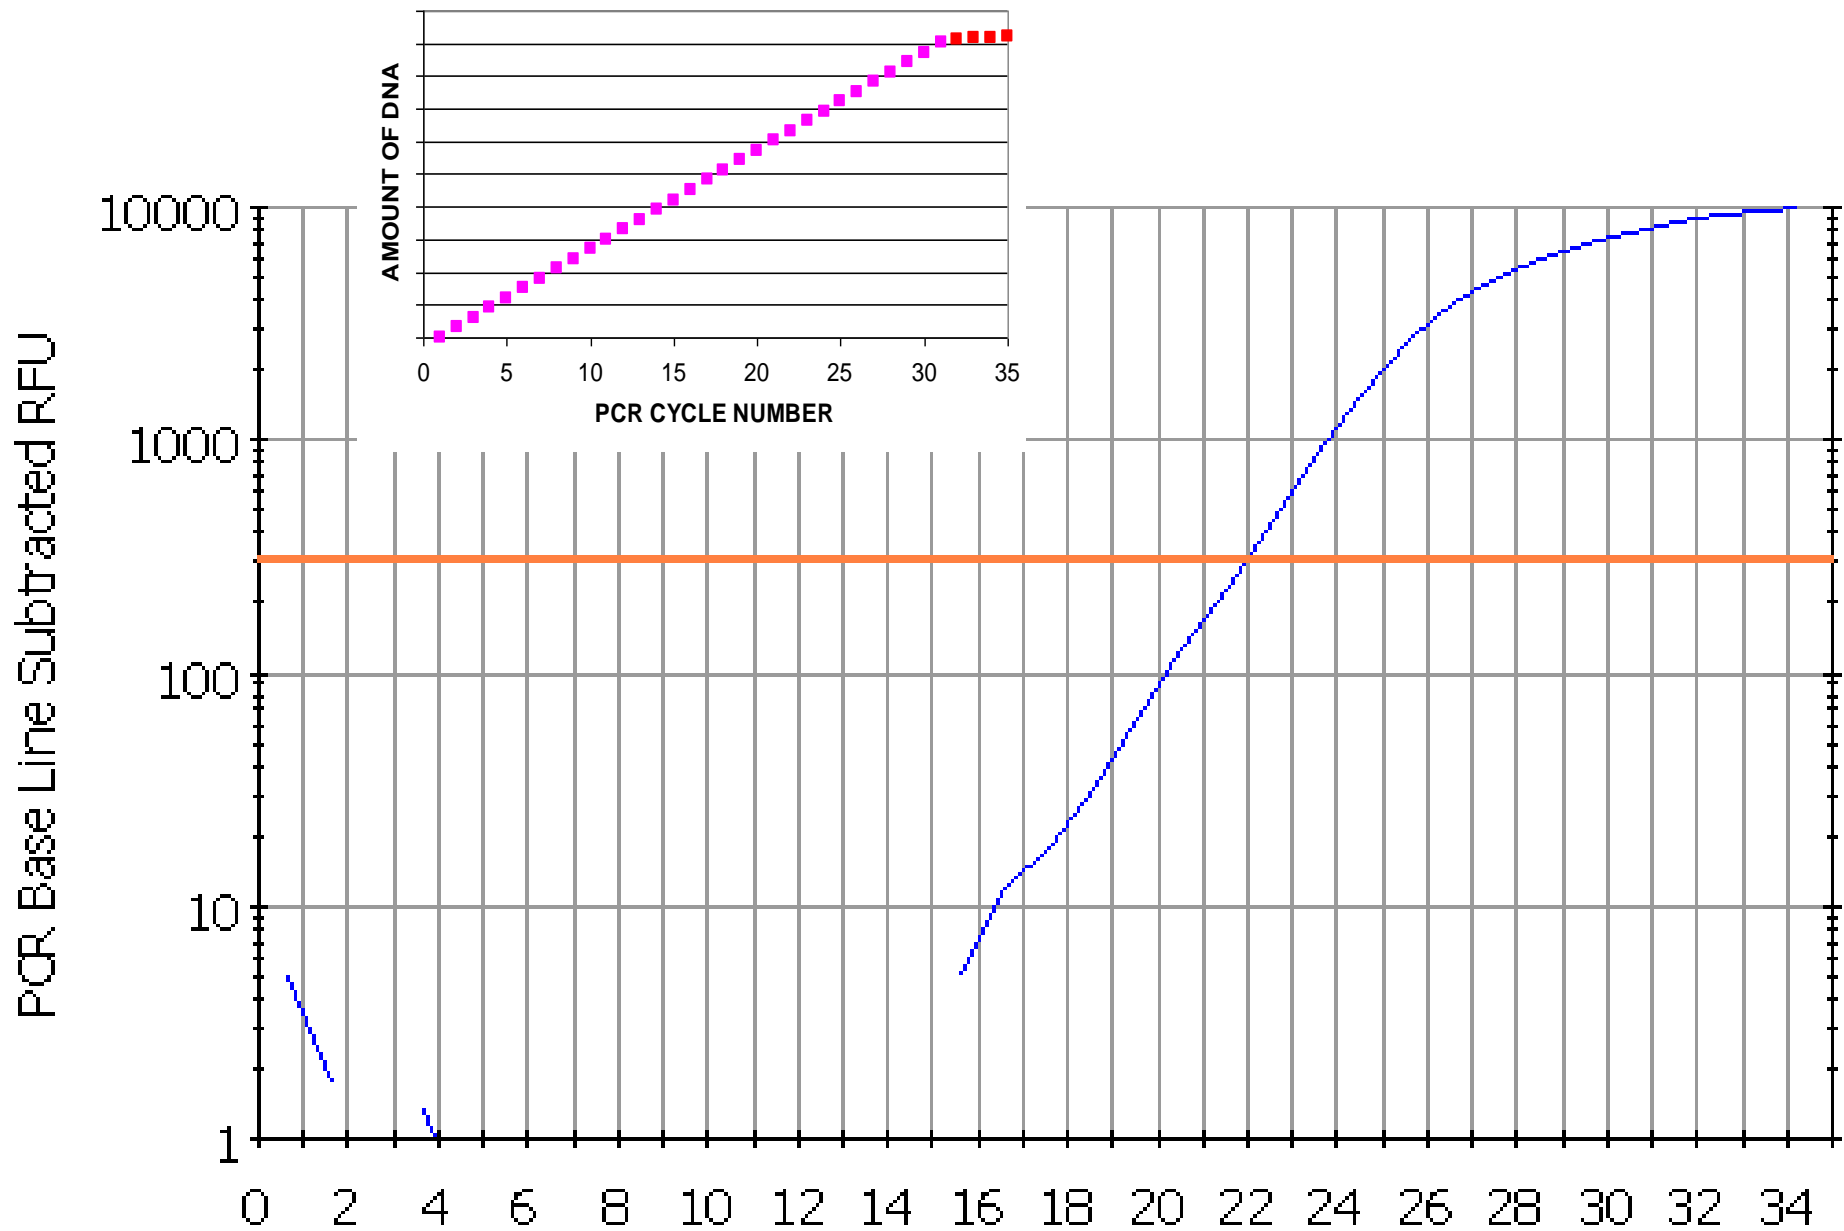


Linear in the range of ~ 20 to ~ 1500

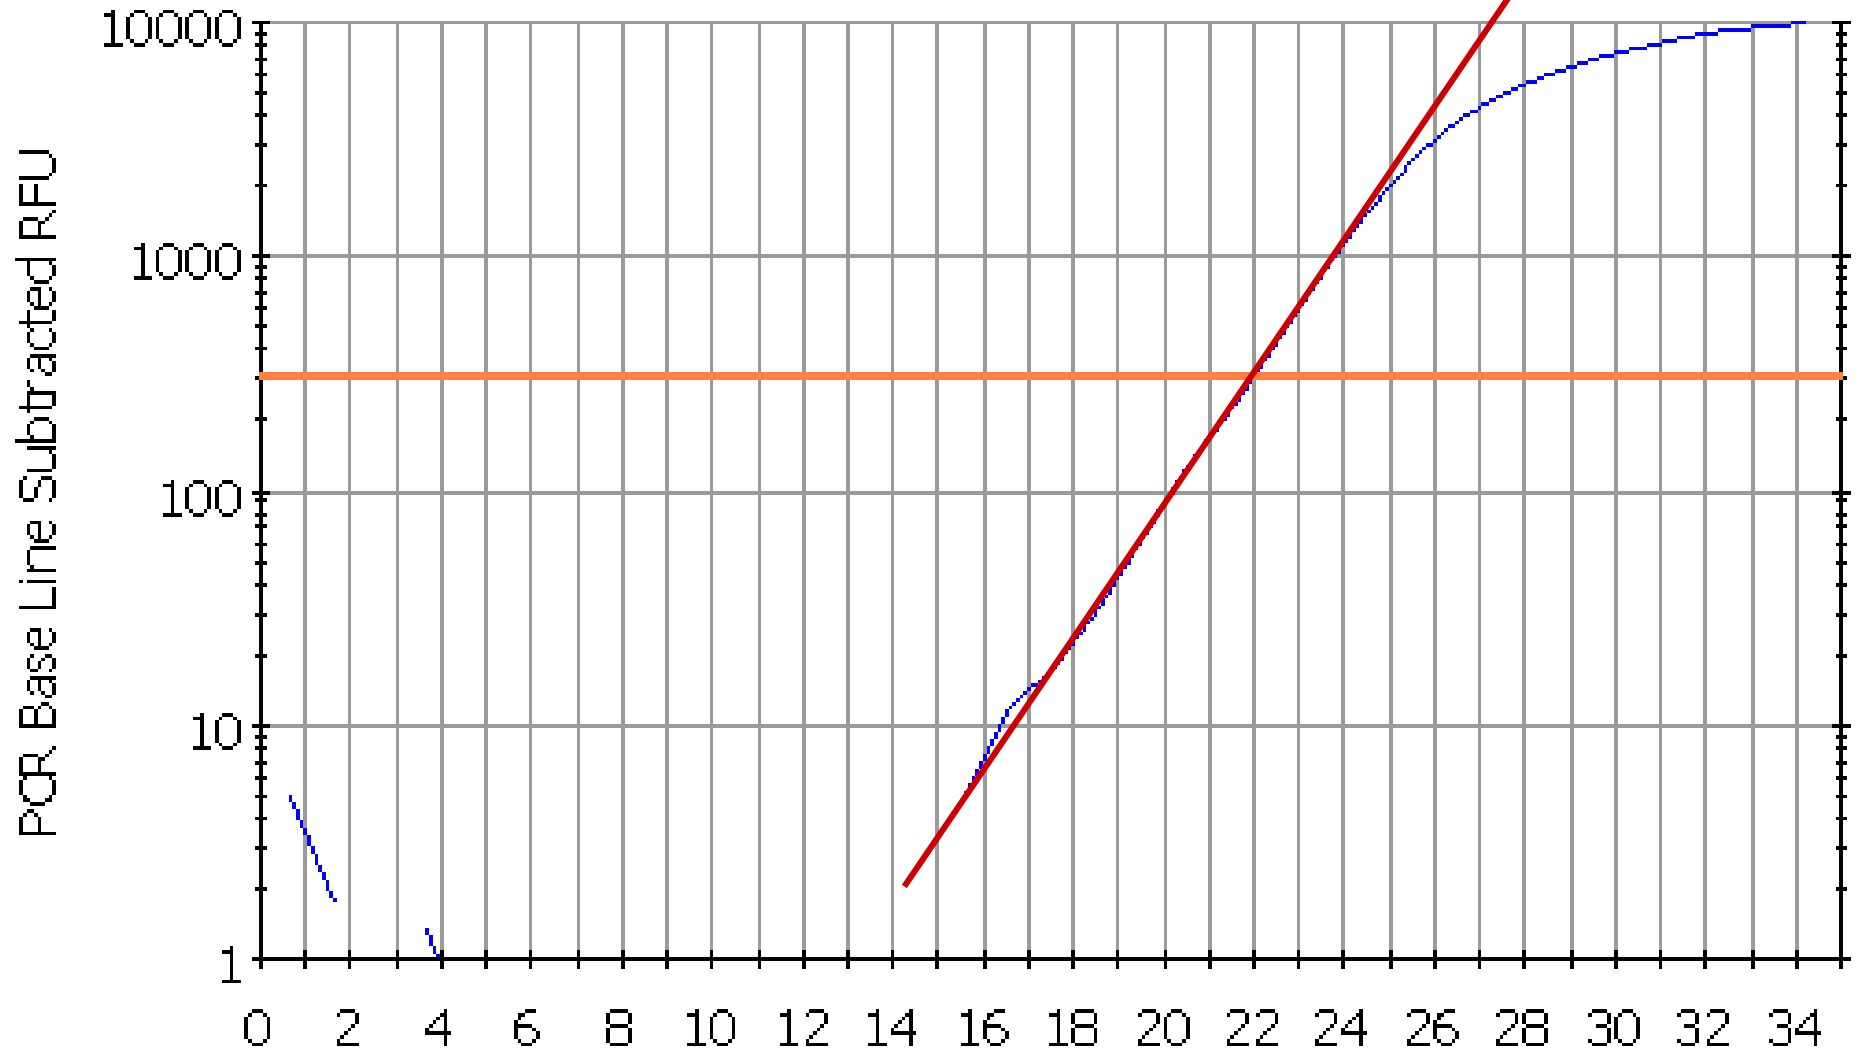


Linear in the range of ~20 to ~1500

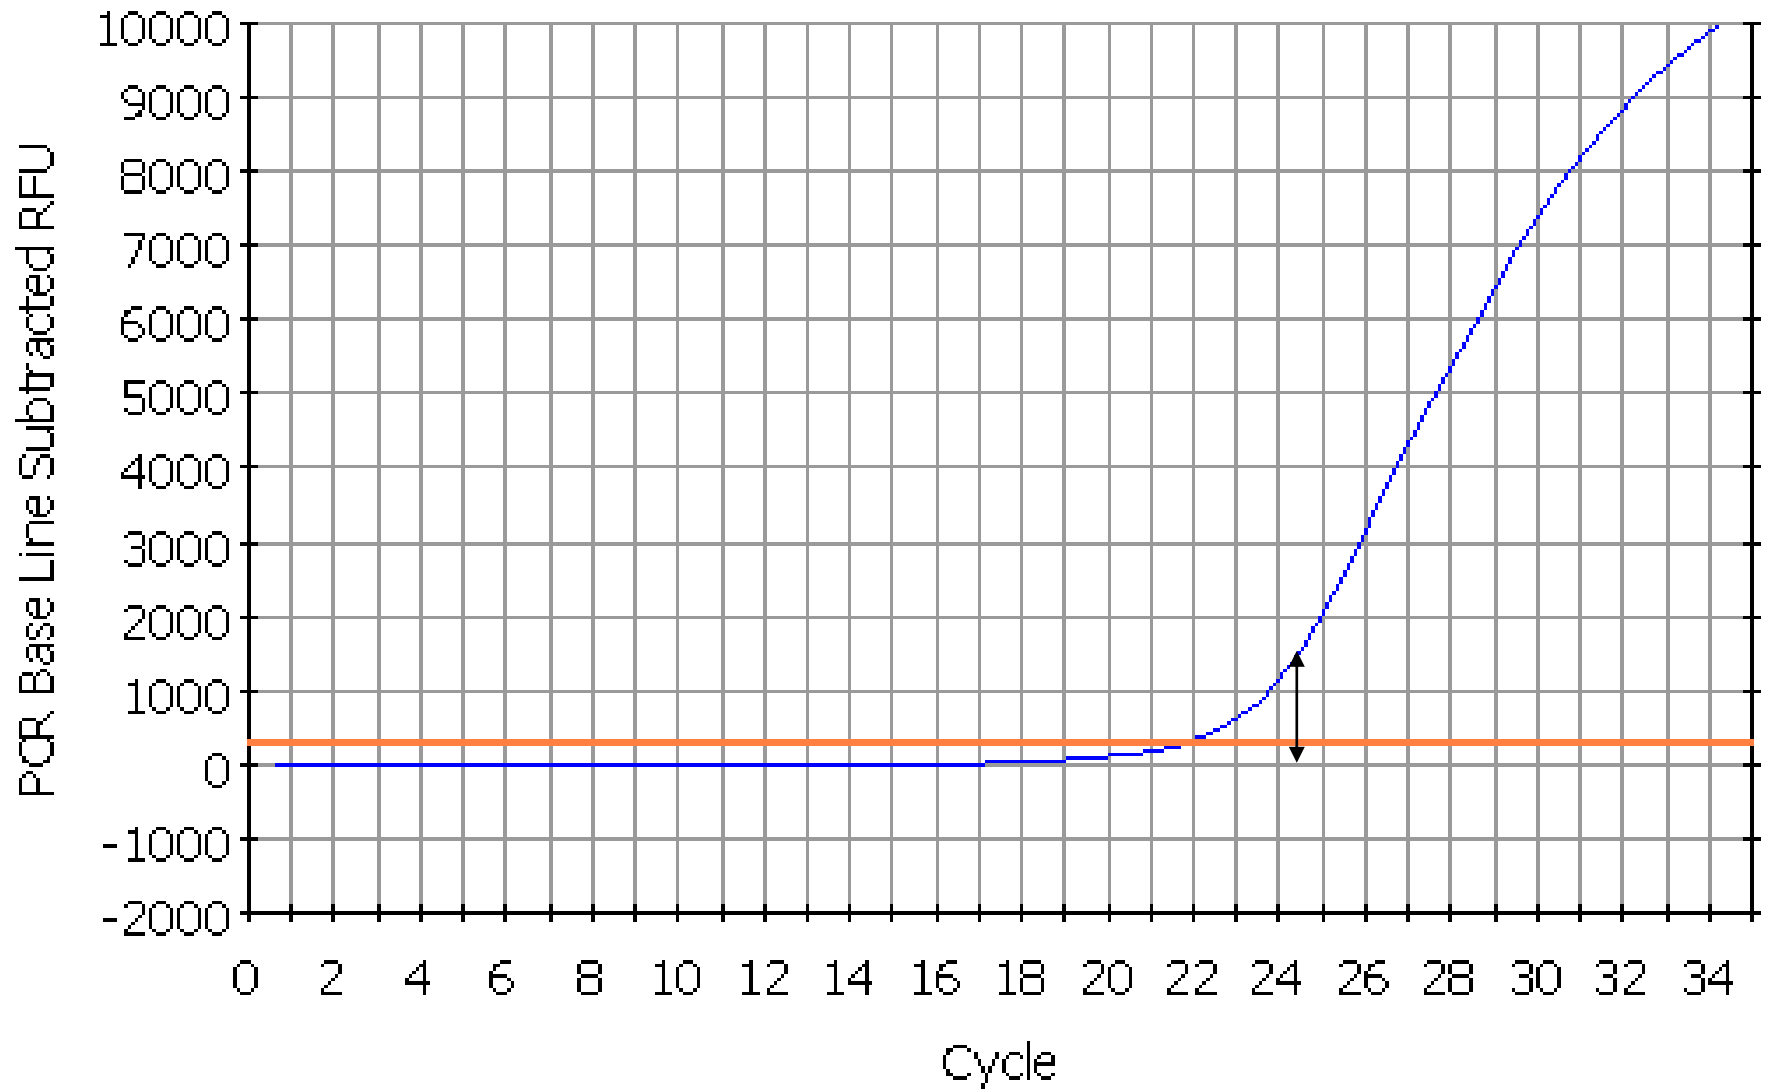


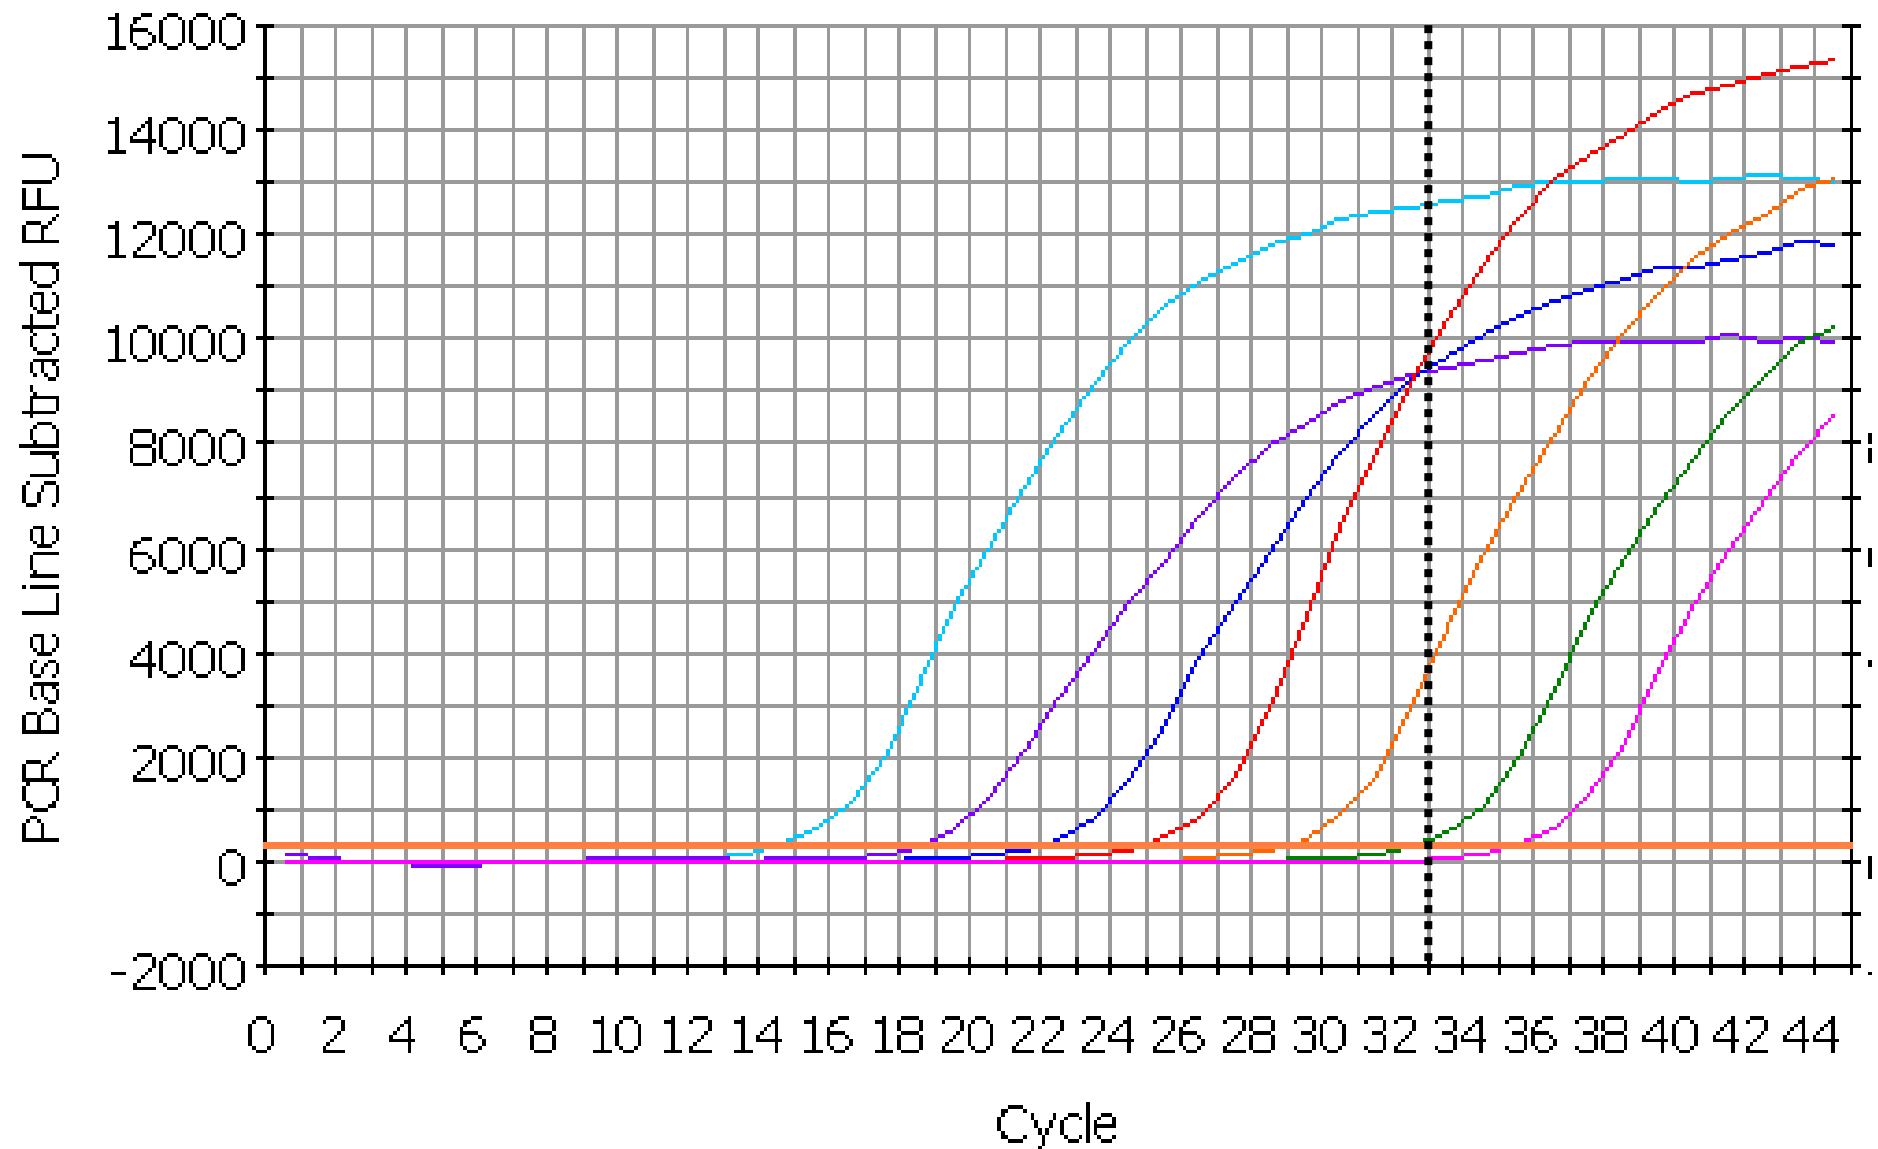


SERIES OF 10-FOLD DILUTIONS

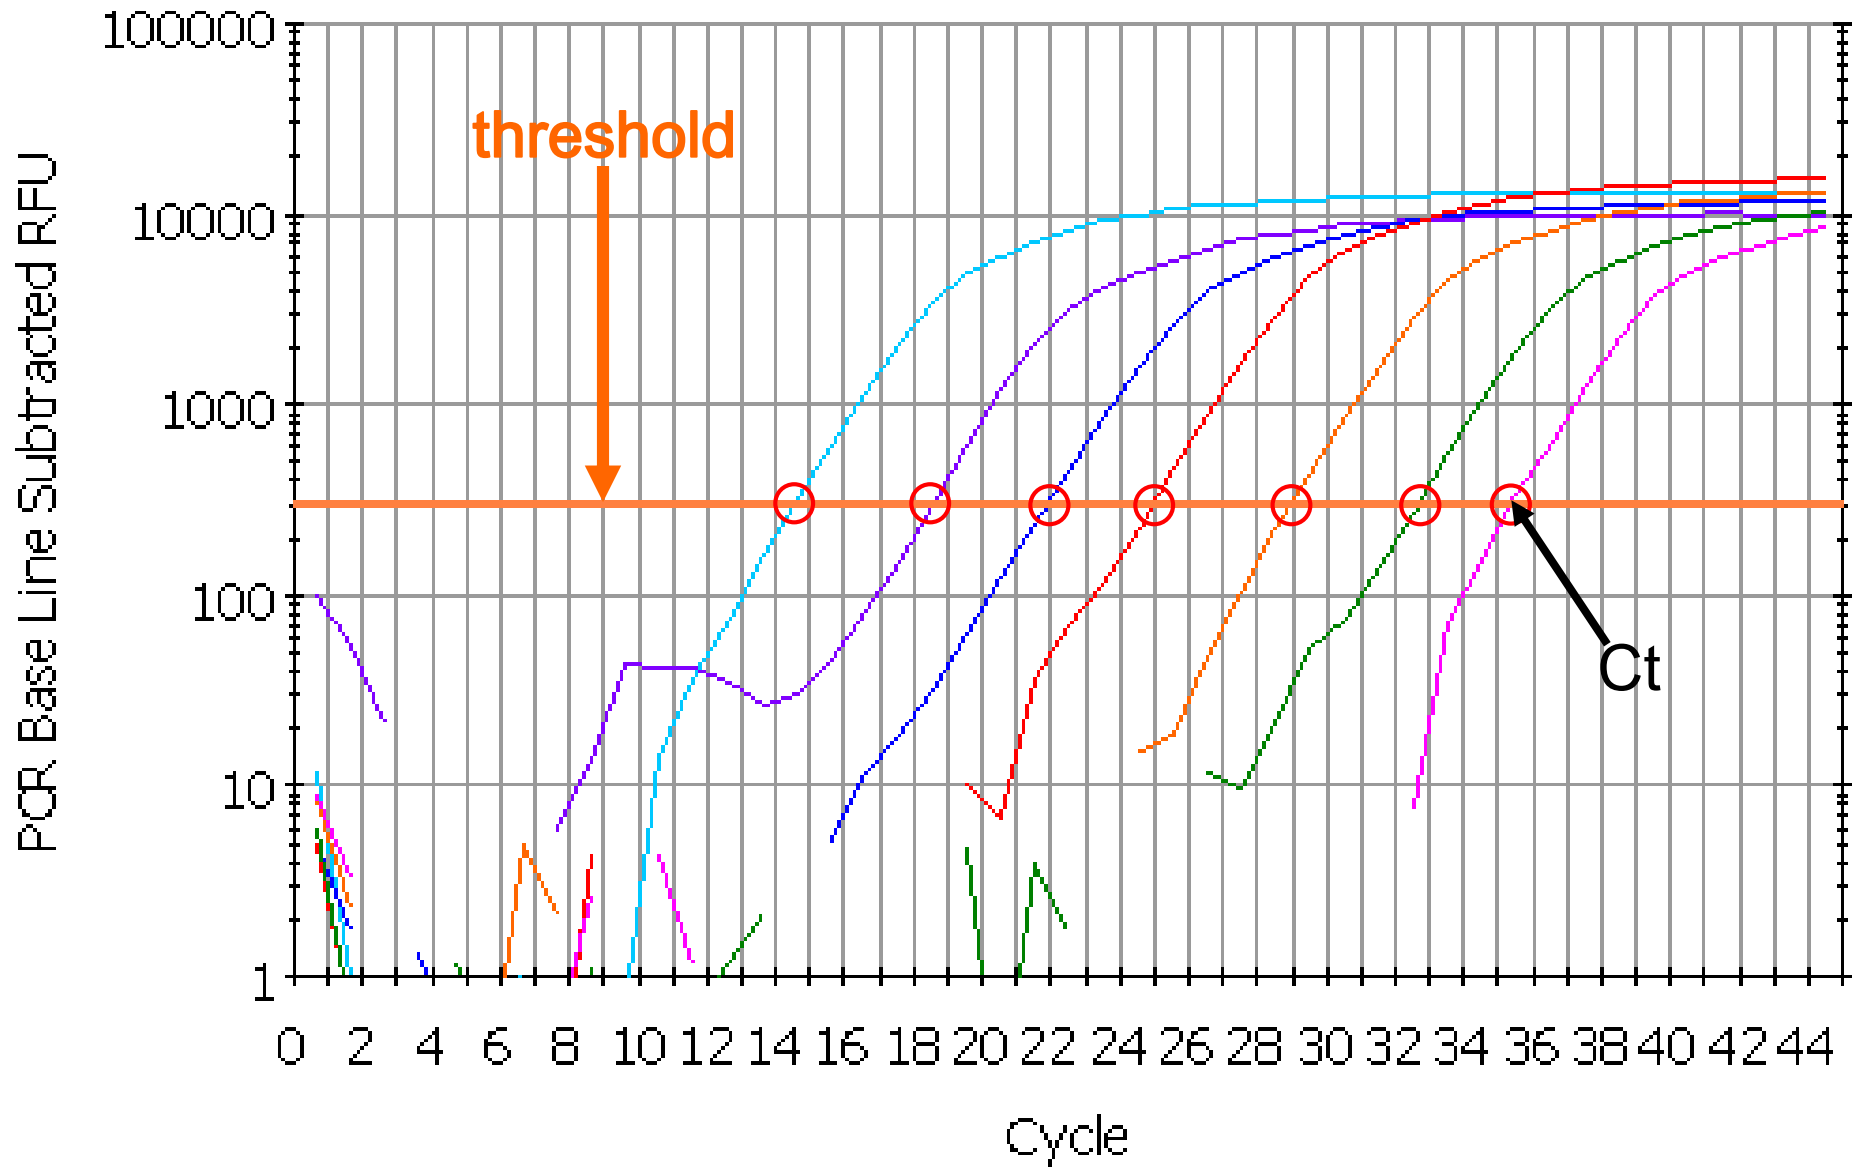

SERIES OF 10-FOLD DILUTIONS

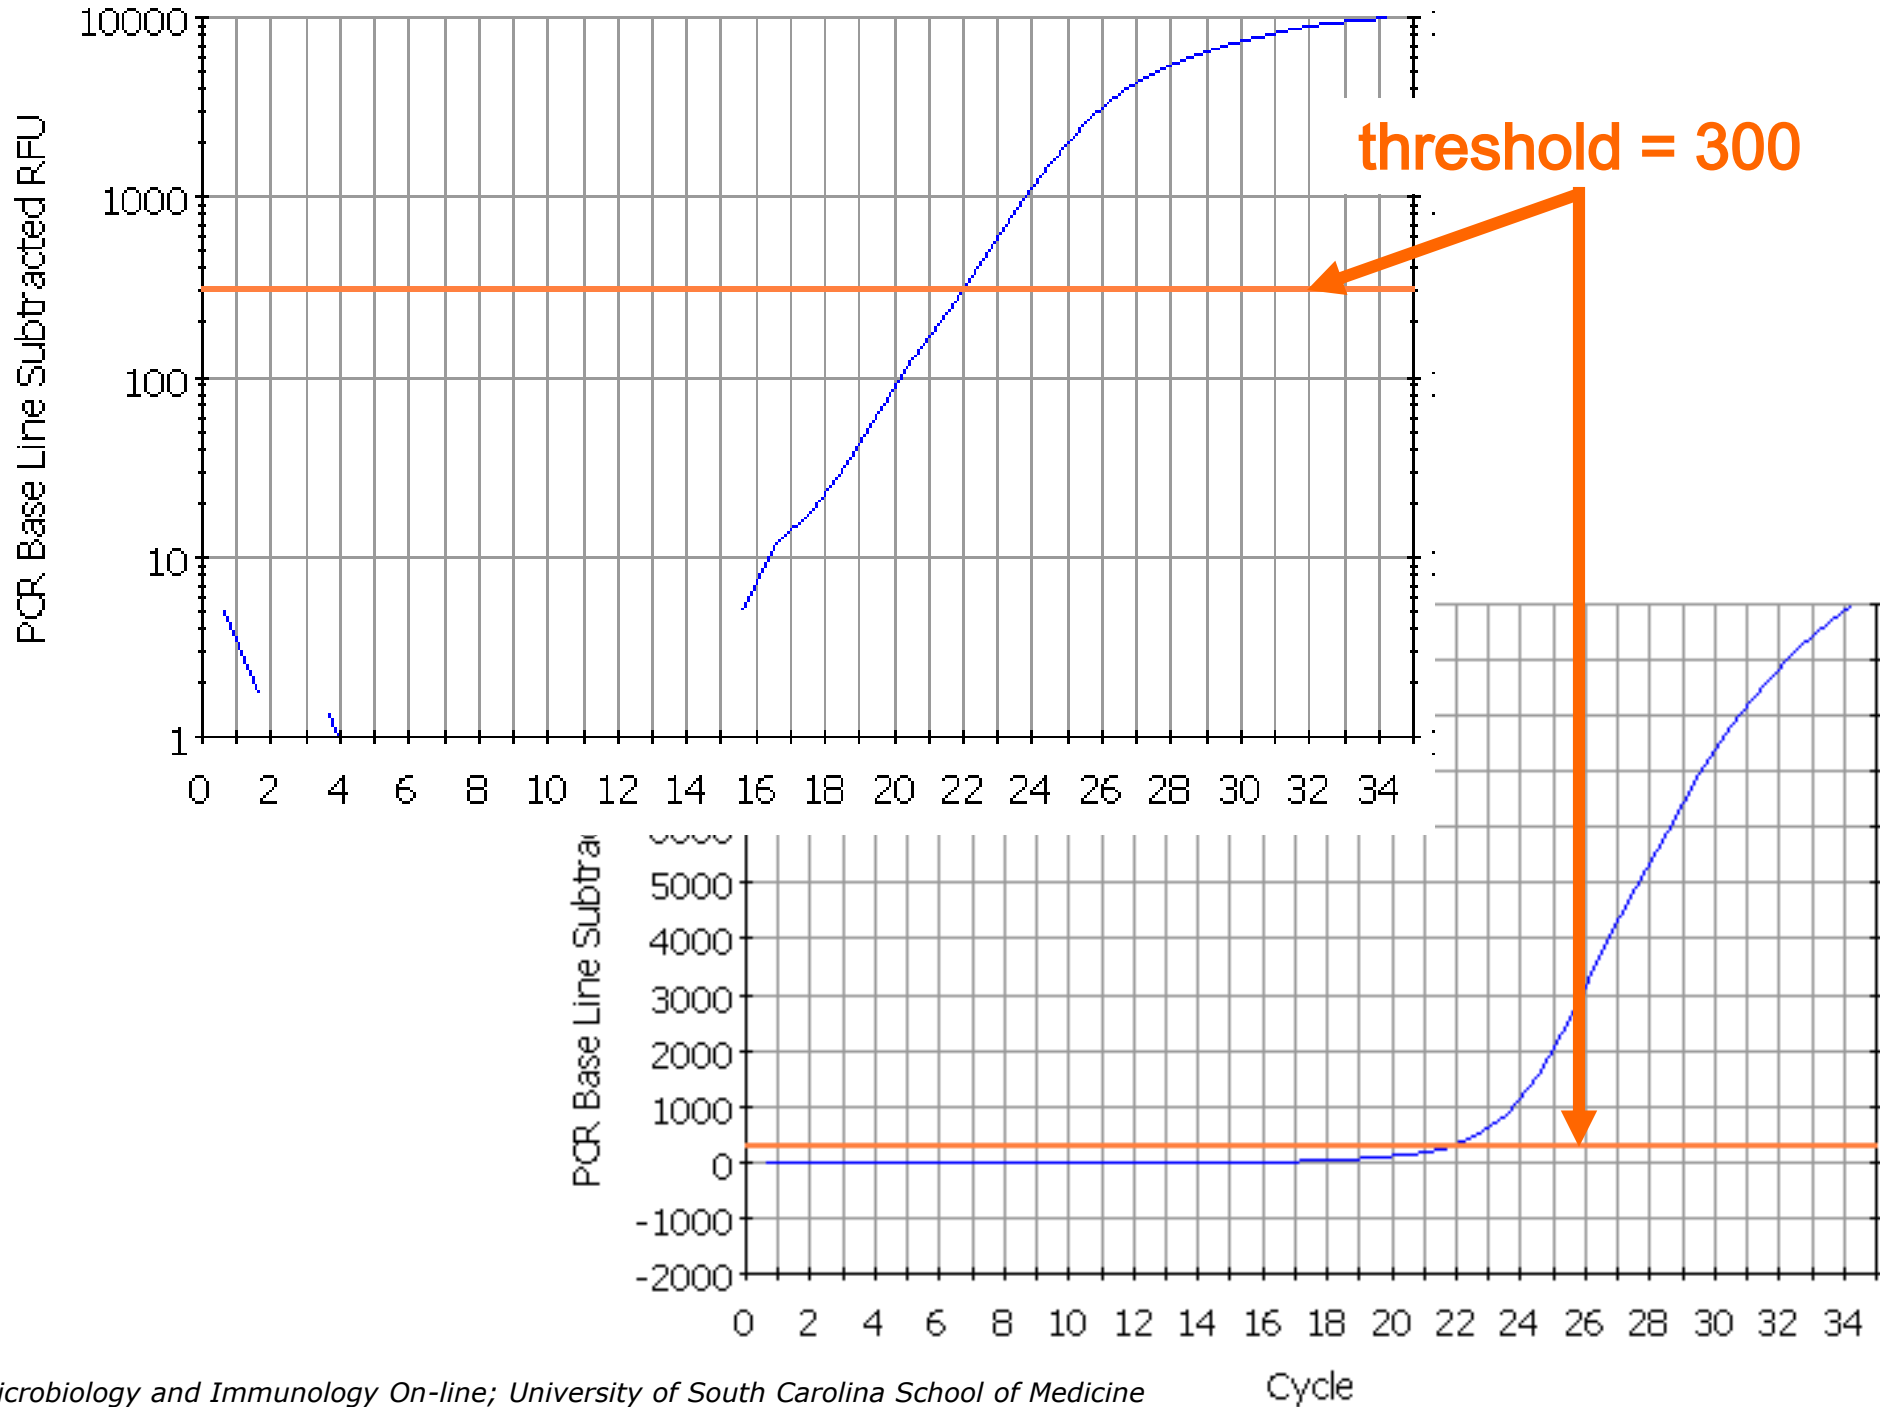

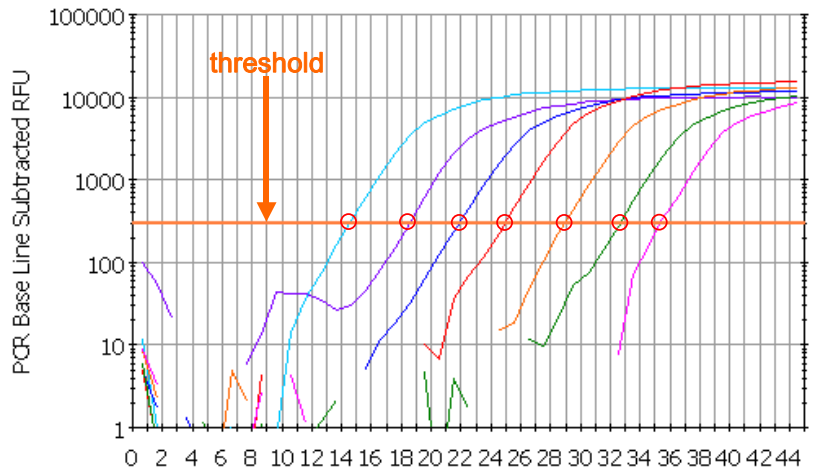

Correlation Coefficient: 0.999 Slope: -3.488 Intercept: 39.204 $Y = -3.488 X + 39.204$


- Unknowns
- Standards




PCR Standard Curve: Data 27-Jan-03 1233ileff.opd

Sensitivity and reproducibility: qPCR vs semi-qPCR


- Dynamic range: up to **9** orders of magnitude (10^9) in qPCR and at most **2** (10^2) in semi-quantitative-PCR
- Variations **inside the** qPCR experiment - up to a few % and in semi-qPCR up to 30-40%
- Variance **between** qPCR experiments - up to a dozen % and in semi-qPCR up to 50-70%
- Detection level in qPCR: about **10** molecules at 50% reproducibility and about **100** molecules at 100% reproducibility.



Sensitivity and reproducibility: qPCR vs semi-qPCR

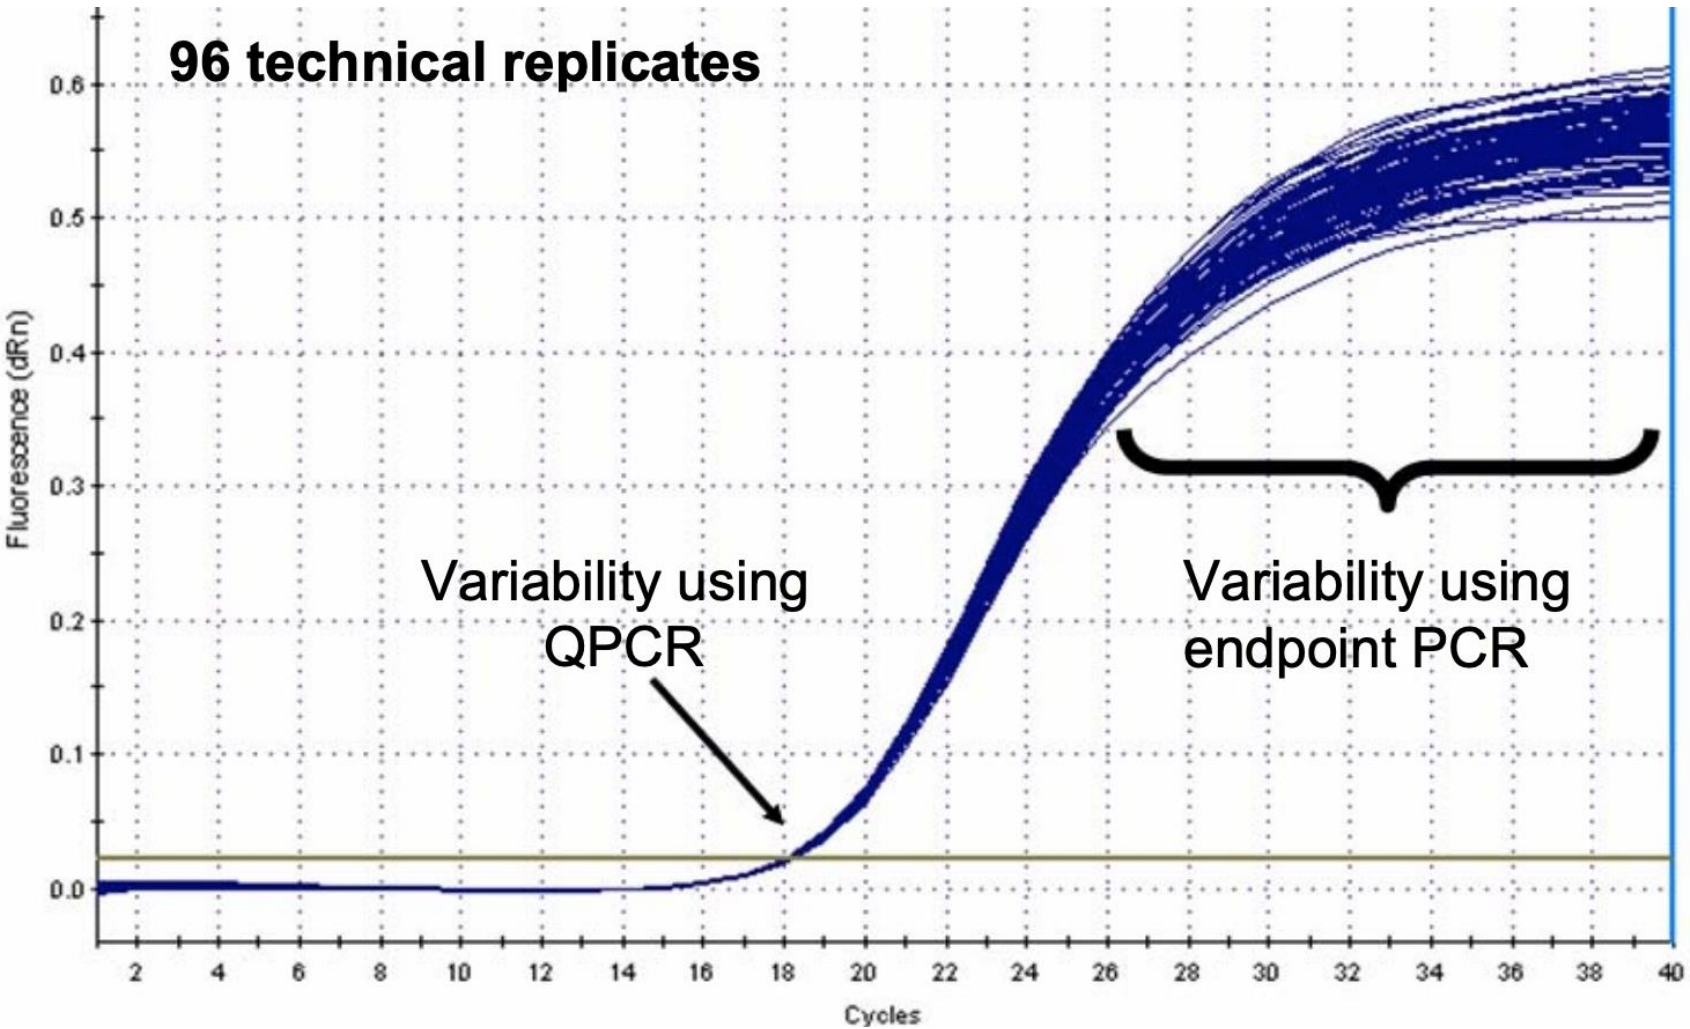

<https://help.medicinalgenomics.com/qpcr-vs-end-point-pcr#>




Different algorithms for determining the value of the threshold cycle

$$C_t = C_p = C_q$$

Threshold
cycle


Maximum of the 2nd
derivative (Roche)

Quantification
cycle



Two methods of quantification


- **"ABSOLUTE QUANTIFICATION" or the method of standard curves.**
- **"RELATIVE QUANTIFICATION"**
- **Both methods are in fact proportional!**




The standard curve method



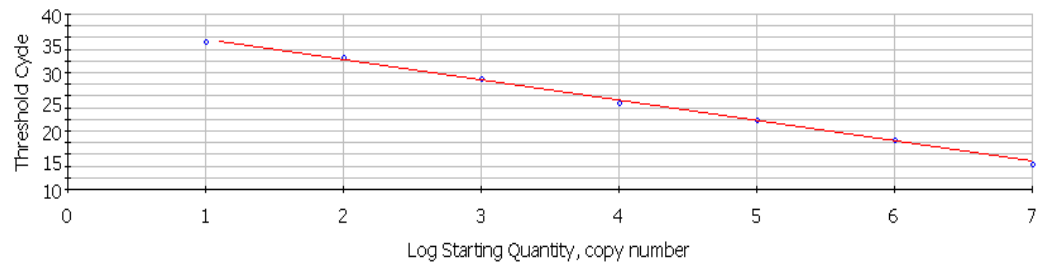




Correlation Coefficient: 0.999 Slope: -3.488 Intercept: 39.204 $Y = -3.488 X + 39.204$

□ Unknowns
♦ Standards



PCR Standard Curve: Data 27-Jan-03 1233ileff.opd



Cursor Standard Unknown Blank + Control - Control Puri


| | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 |
|---|---|---|---|----|----|----|----|----|---|
| A | | | | | | | | | |
| B | | 1 | 2 | 3 | 4 | 5 | 6 | 7 | — |
| C | | C | C | C | | E | E | E | |
| D | | | | | | | | | |
| E | | 8 | 9 | 10 | 11 | 12 | 13 | 14 | — |
| F | | C | C | C | | E | E | E | |
| G | | | | | | | | | |

← dilutions target DNA
 ← triplicates cDNA
 ← DNA reference dilutions
 ← triplicates cDNA


} target primers
 } reference primers

Correlation Coefficient: 0.999 Slope: -3.488 Intercept: 39.204 $Y = -3.488 X + 39.204$

□ Unknowns
○ Standards

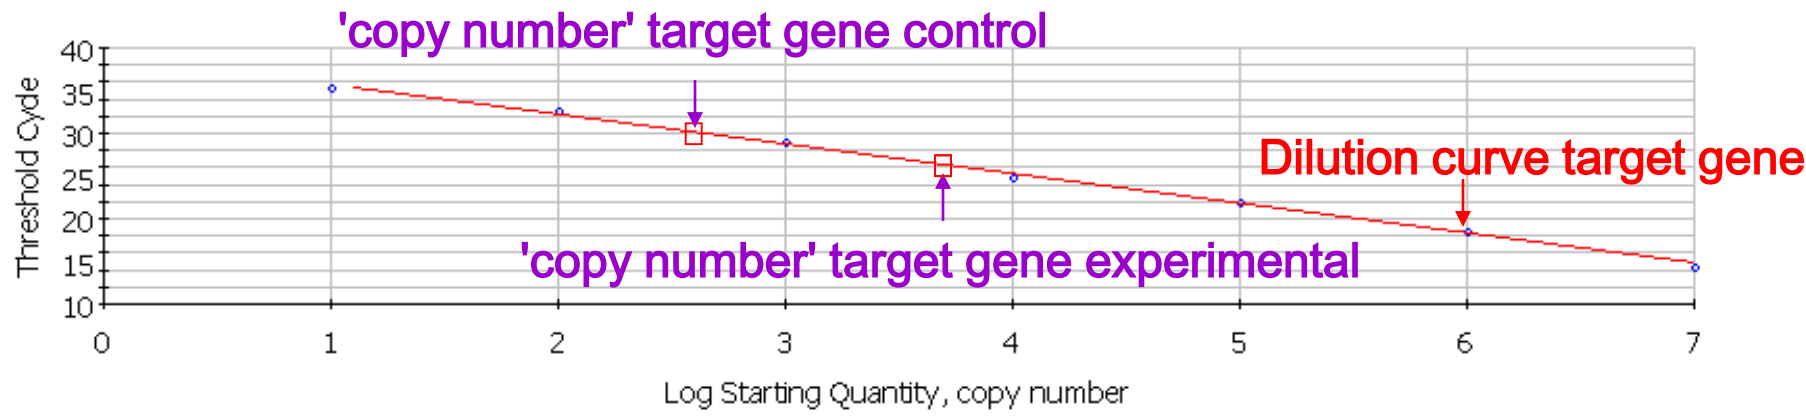

NORTHERN

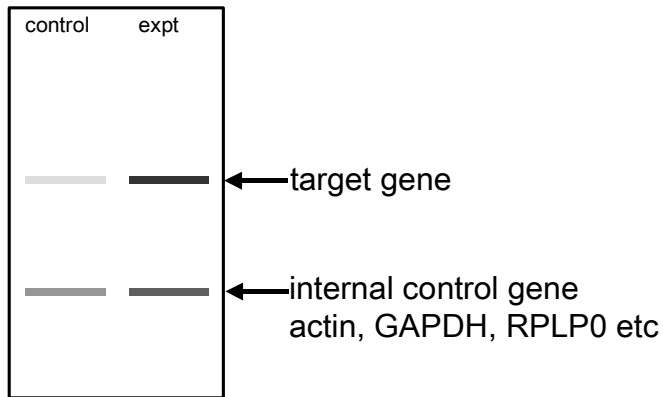


fold change in target gene = $\frac{\text{copy number experimental}}{\text{copy number control}}$


Ratio experimental/control = $\frac{\text{fold change in target gene}}{\text{fold change in reference gene}}$

Correlation Coefficient: 1.000 Slope: -3.360 Intercept: 39.319 $Y = -3.360 X + 39.319$

□ Unknowns
● Standards

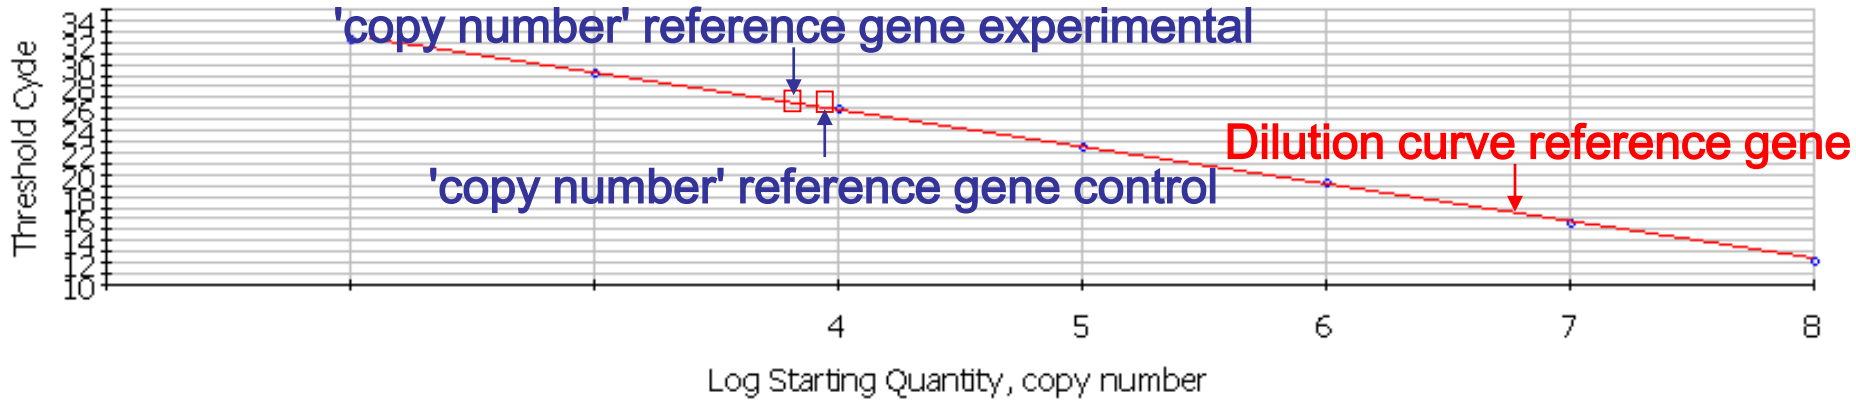


NORTHERN

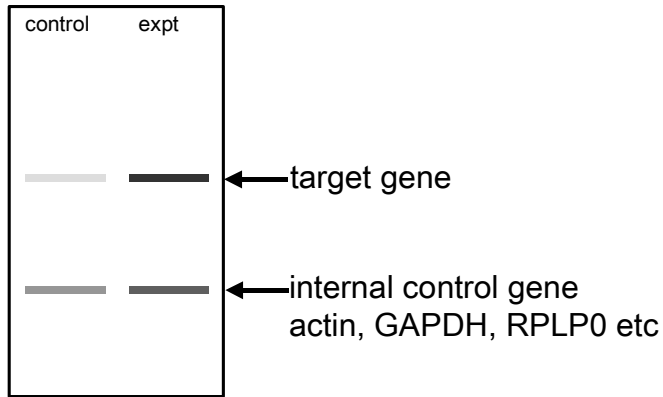

$$\text{Ratio experimental/control} = \frac{\text{fold change in target gene}}{\text{fold change in reference gene}}$$

| | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 |
|---|---|---|---|----|----|----|----|----|---|
| A | | | | | | | | | |
| B | | 1 | 2 | 3 | 4 | 5 | 6 | 7 | — |
| C | | C | C | C | | E | E | E | |
| D | | | | | | | | | |
| E | | 8 | 9 | 10 | 11 | 12 | 13 | 14 | — |
| F | | C | C | C | | E | E | E | |
| G | | | | | | | | | |

Efficiency is a key factor of the qPCR reaction



| CYCLE | AMOUNT OF DNA 100% EFFICIENCY | AMOUNT OF DNA 90% EFFICIENCY | AMOUNT OF DNA 80% EFFICIENCY | AMOUNT OF DNA 70% EFFICIENCY |
|-------|----------------------------------|---------------------------------|---------------------------------|---------------------------------|
| 0 | 1 | 1 | 1 | 1 |
| 1 | 2 | 2 | 2 | 2 |
| 2 | 4 | 4 | 3 | 3 |
| 3 | 8 | 7 | 6 | 5 |
| 4 | 16 | 13 | 10 | 8 |
| 5 | 32 | 25 | 19 | 14 |
| 6 | 64 | 47 | 34 | 24 |
| 7 | 128 | 89 | 61 | 41 |
| 8 | 256 | 170 | 110 | 70 |
| 9 | 512 | 323 | 198 | 119 |
| 10 | 1,024 | 613 | 357 | 202 |
| 11 | 2,048 | 1,165 | 643 | 343 |
| 12 | 4,096 | 2,213 | 1,157 | 583 |
| 13 | 8,192 | 4,205 | 2,082 | 990 |
| 14 | 16,384 | 7,990 | 3,748 | 1,684 |
| 15 | 32,768 | 15,181 | 6,747 | 2,862 |
| 16 | 65,536 | 28,844 | 12,144 | 4,866 |
| 17 | 131,072 | 54,804 | 21,859 | 8,272 |
| 18 | 262,144 | 104,127 | 39,346 | 14,063 |
| 19 | 524,288 | 197,842 | 70,824 | 23,907 |
| 20 | 1,048,576 | 375,900 | 127,482 | 40,642 |
| 21 | 2,097,152 | 714,209 | 229,468 | 69,092 |
| 22 | 4,194,304 | 1,356,998 | 413,043 | 117,456 |
| 23 | 8,388,608 | 2,578,296 | 743,477 | 199,676 |
| 24 | 16,777,216 | 4,898,763 | 1,338,259 | 339,449 |
| 25 | 33,554,432 | 9,307,650 | 2,408,866 | 577,063 |
| 26 | 67,108,864 | 17,684,534 | 4,335,959 | 981,007 |
| 27 | 134,217,728 | 33,600,615 | 7,804,726 | 1,667,711 |
| 28 | 268,435,456 | 63,841,168 | 14,048,506 | 2,835,109 |
| 29 | 536,870,912 | 121,298,220 | 25,287,311 | 4,819,686 |
| 30 | 1,073,741,824 | 230,466,618 | 45,517,160 | 8,193,466 |

AFTER 1 CYCLE

100% = 2.00x

90% = 1.90x

80% = 1.80x

70% = 1.70x

| CYCLE | AMOUNT OF DNA 100% EFFICIENCY | AMOUNT OF DNA 90% EFFICIENCY | AMOUNT OF DNA 80% EFFICIENCY | AMOUNT OF DNA 70% EFFICIENCY |
|-------|----------------------------------|---------------------------------|---------------------------------|---------------------------------|
| 0 | 1 | 1 | 1 | 1 |
| 1 | 2 | 2 | 2 | 2 |
| 2 | 4 | 4 | 3 | 3 |
| 3 | 8 | 7 | 6 | 5 |
| 4 | 16 | 13 | 10 | 8 |
| 5 | 32 | 25 | 19 | 14 |
| 6 | 64 | 47 | 34 | 24 |
| 7 | 128 | 89 | 61 | 41 |
| 8 | 256 | 170 | 110 | 70 |
| 9 | 512 | 323 | 198 | 119 |
| 10 | 1,024 | 613 | 357 | 202 |
| 11 | 2,048 | 1,165 | 643 | 343 |
| 12 | 4,096 | 2,213 | 1,157 | 583 |
| 13 | 8,192 | 4,205 | 2,082 | 990 |
| 14 | 16,384 | 7,990 | 3,748 | 1,684 |
| 15 | 32,768 | 15,181 | 6,747 | 2,862 |
| 16 | 65,536 | 28,844 | 12,144 | 4,866 |
| 17 | 131,072 | 54,804 | 21,859 | 8,272 |
| 18 | 262,144 | 104,127 | 39,346 | 14,063 |
| 19 | 524,288 | 197,842 | 70,824 | 23,907 |
| 20 | 1,048,576 | 375,900 | 127,482 | 40,642 |
| 21 | 2,097,152 | 714,209 | 229,468 | 69,092 |
| 22 | 4,194,304 | 1,356,998 | 413,043 | 117,456 |
| 23 | 8,388,608 | 2,578,296 | 743,477 | 199,676 |
| 24 | 16,777,216 | 4,898,763 | 1,338,259 | 339,449 |
| 25 | 33,554,432 | 9,307,650 | 2,408,866 | 577,063 |
| 26 | 67,108,864 | 17,684,534 | 4,335,959 | 981,007 |
| 27 | 134,217,728 | 33,600,615 | 7,804,726 | 1,667,711 |
| 28 | 268,435,456 | 63,841,168 | 14,048,506 | 2,835,109 |
| 29 | 536,870,912 | 121,298,220 | 25,287,311 | 4,819,686 |
| 30 | 1,073,741,824 | 230,466,618 | 45,517,160 | 8,193,466 |

AFTER 1 CYCLE

100% = 2.00x

90% = 1.90x



80% = 1.80x


70% = 1.70x


AFTER N CYCLES:

**fold increase =
(efficiency)ⁿ**


| CYCLE | AMOUNT OF DNA | AMOUNT OF DNA | AMOUNT OF DNA | AMOUNT OF DNA |
|-------|-----------------|----------------|----------------|----------------|
| | 100% EFFICIENCY | 90% EFFICIENCY | 80% EFFICIENCY | 70% EFFICIENCY |
| 0 | 1 | 1 | 1 | 1 |
| 1 | 2 | 2 | 2 | 2 |
| 2 | 4 | 4 | 3 | 3 |
| 3 | 8 | 7 | 6 | 5 |
| 4 | 16 | 13 | 10 | 8 |
| 5 | 32 | 25 | 19 | 14 |
| 6 | 64 | 47 | 34 | 24 |
| 7 | 128 | 89 | 61 | 41 |
| 8 | 256 | 170 | 110 | 70 |
| 9 | 512 | 323 | 198 | 119 |
| 10 | 1,024 | 613 | 357 | 202 |
| 11 | 2,048 | 1,165 | 643 | 343 |
| 12 | 4,096 | 2,213 | 1,157 | 583 |
| 13 | 8,192 | 4,205 | 2,082 | 990 |
| 14 | 16,384 | 7,990 | 3,748 | 1,684 |
| 15 | 32,768 | 15,181 | 6,747 | 2,862 |
| 16 | 65,536 | 28,844 | 12,144 | 4,866 |
| 17 | 131,072 | 54,804 | 21,859 | 8,272 |
| 18 | 262,144 | 104,127 | 39,346 | 14,063 |
| 19 | 524,288 | 197,842 | 70,824 | 23,907 |
| 20 | 1,048,576 | 375,900 | 127,482 | 40,642 |
| 21 | 2,097,152 | 714,209 | 229,468 | 69,092 |
| 22 | 4,194,304 | 1,356,998 | 413,043 | 117,456 |
| 23 | 8,388,608 | 2,578,296 | 743,477 | 199,676 |
| 24 | 16,777,216 | 4,898,763 | 1,338,259 | 339,449 |
| 25 | 33,554,432 | 9,307,650 | 2,408,866 | 577,063 |
| 26 | 67,108,864 | 17,684,534 | 4,335,959 | 981,007 |
| 27 | 134,217,728 | 33,600,615 | 7,804,726 | 1,667,711 |
| 28 | 268,435,456 | 63,841,168 | 14,048,506 | 2,835,109 |
| 29 | 536,870,912 | 121,298,220 | 25,287,311 | 4,819,686 |
| 30 | 1,073,741,824 | 230,466,618 | 45,517,160 | 8,193,466 |

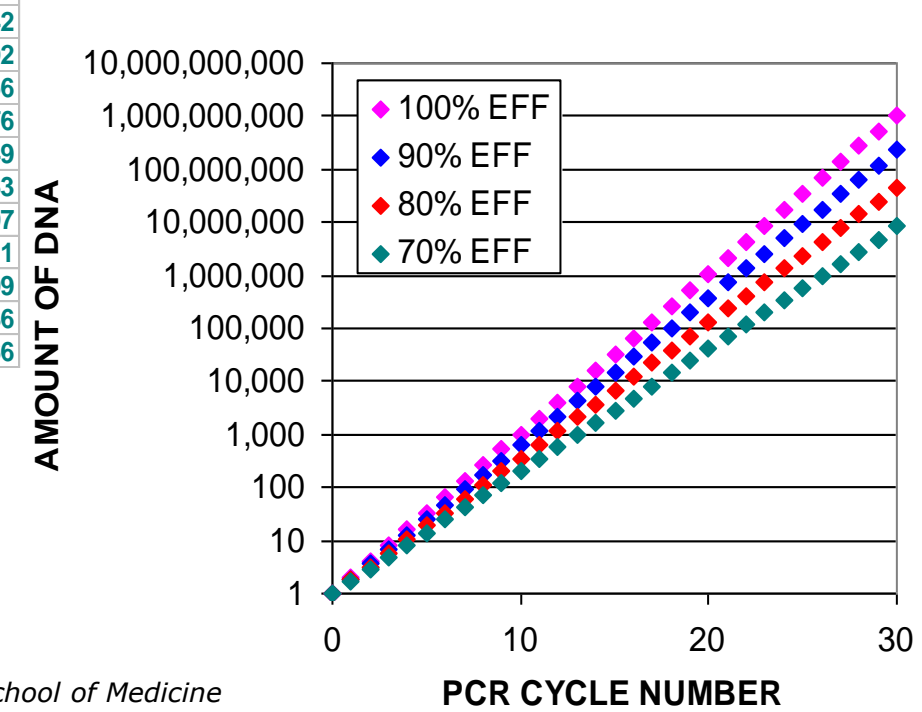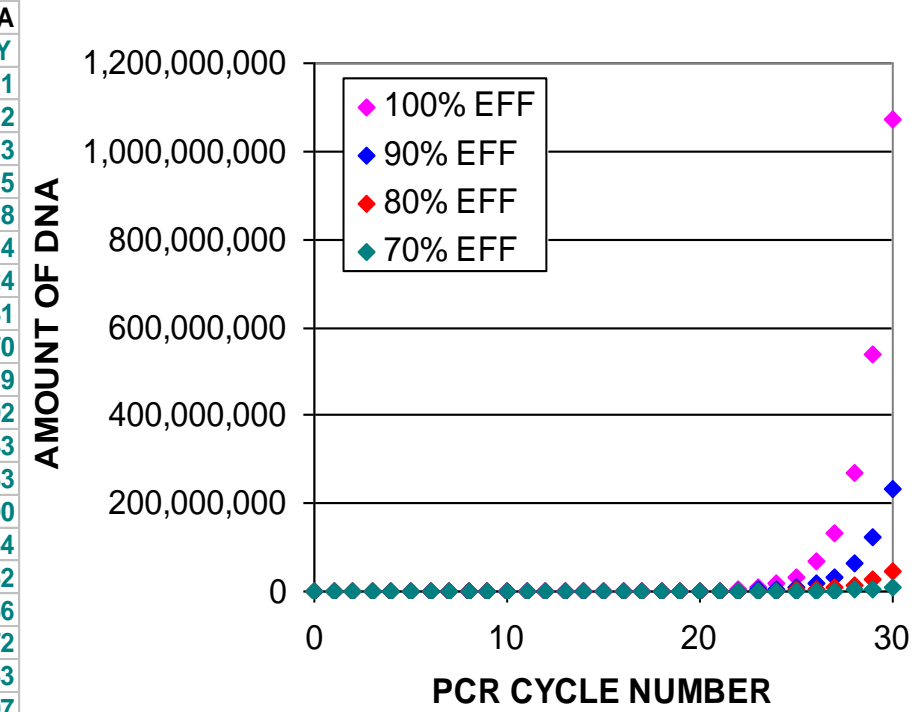

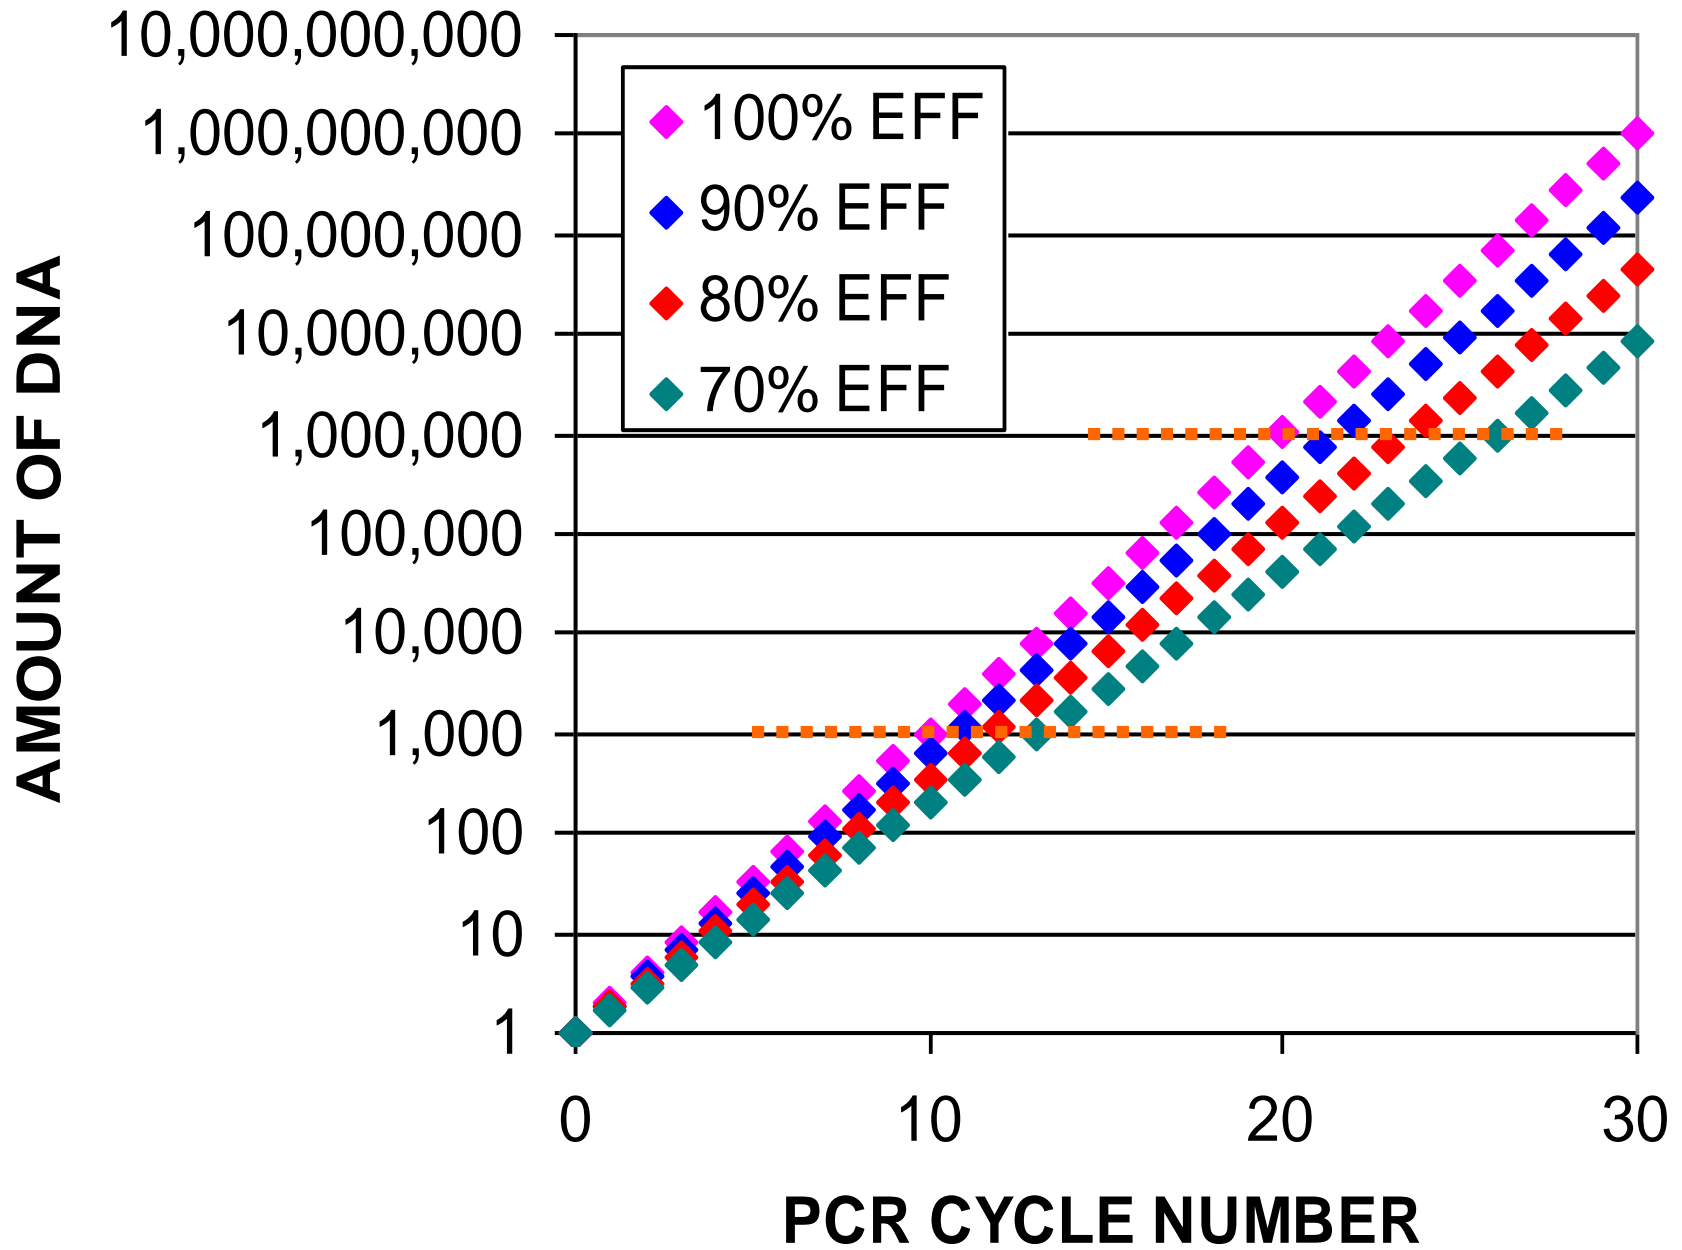

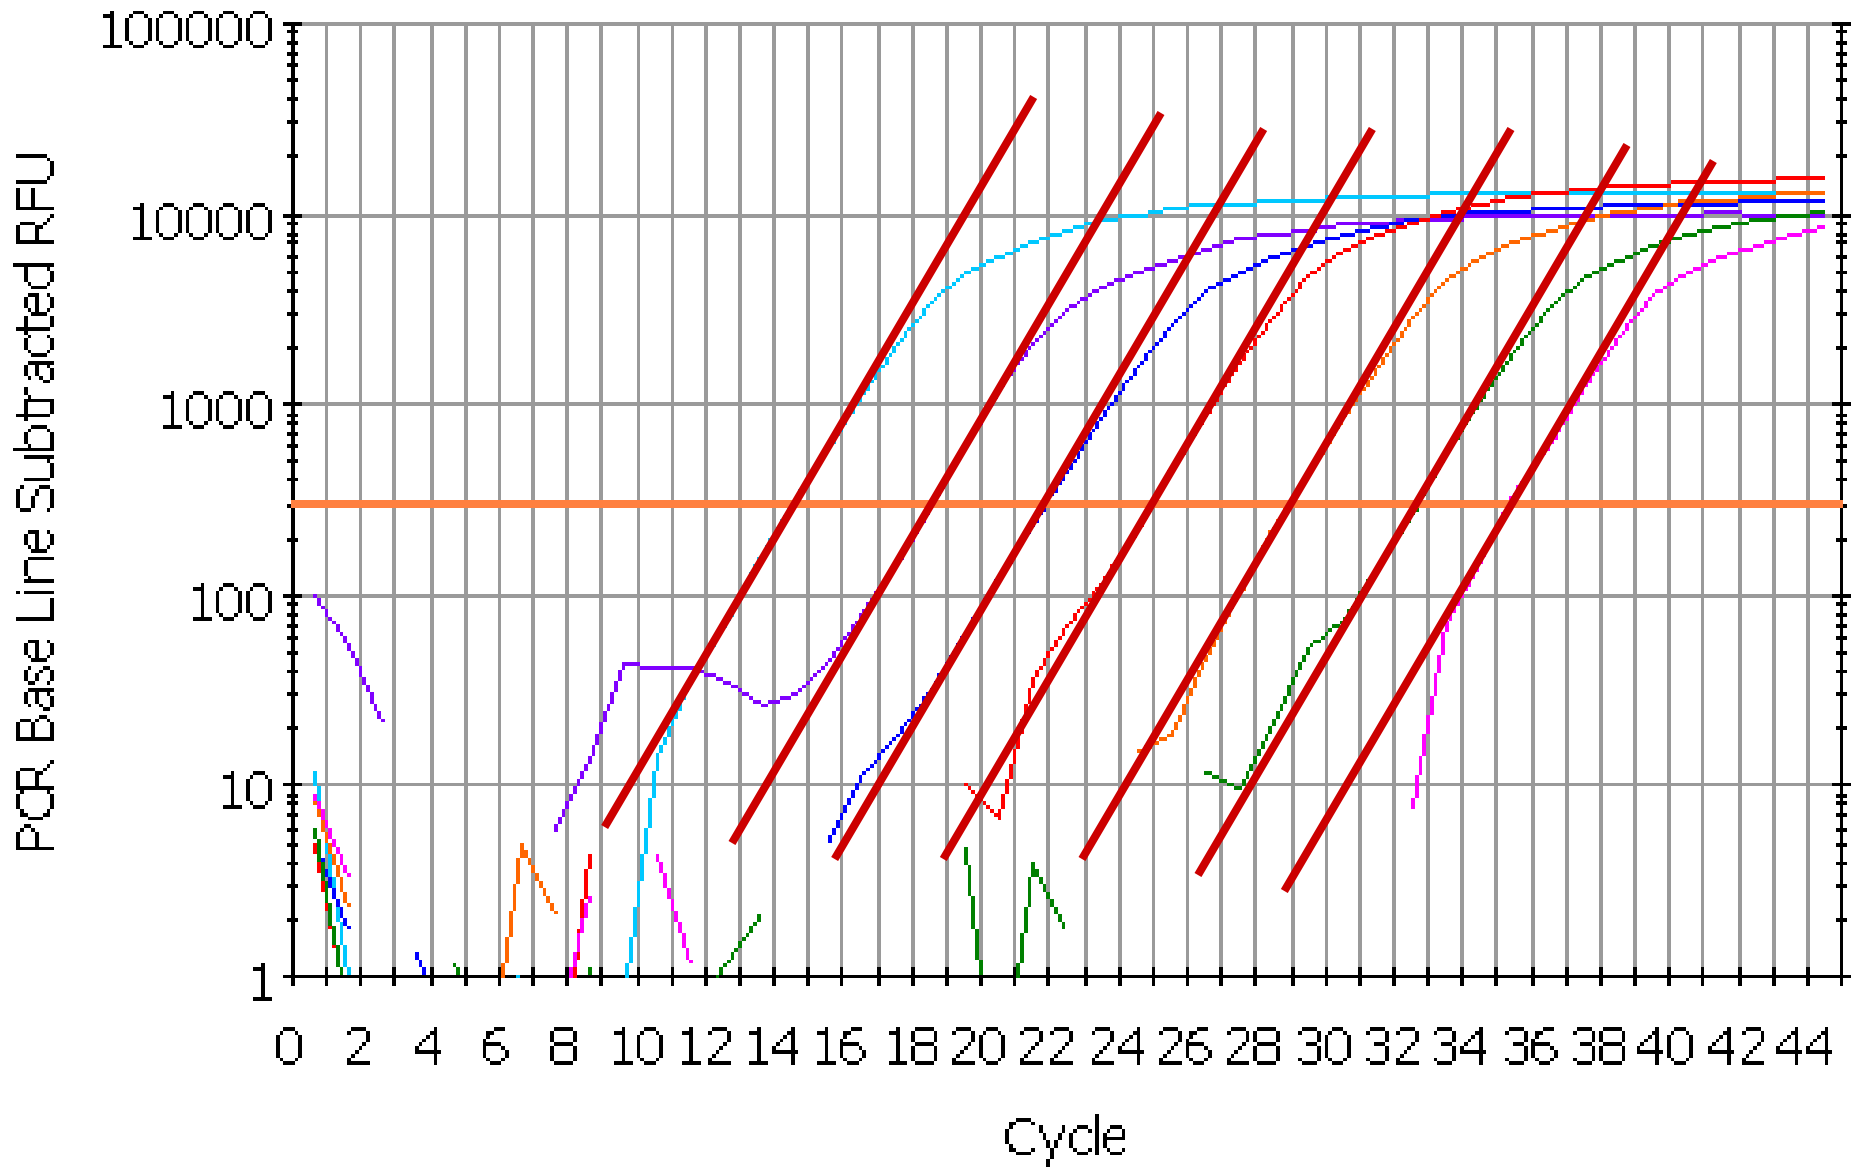

SERIES OF 10-FOLD DILUTIONS

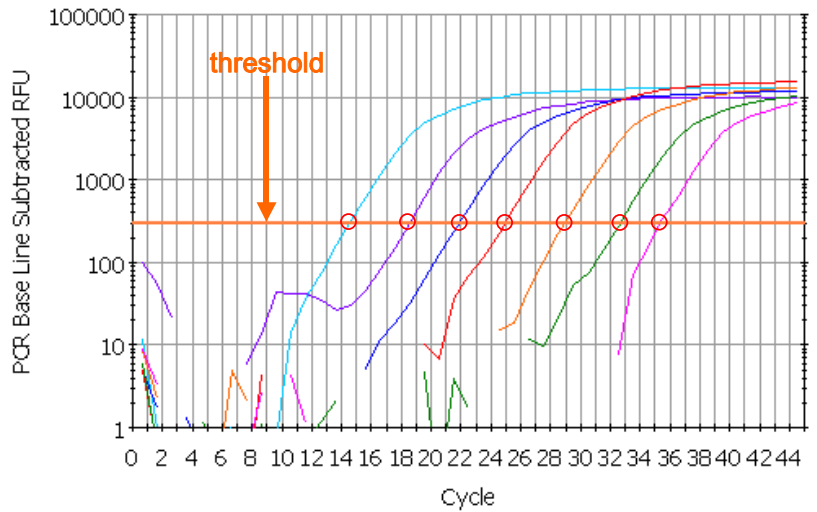

Correlation Coefficient: 0.999 Slope: -3.488 Intercept: 39.204 $Y = -3.488 X + 39.204$
 PCR Efficiency: 93.5 %

□ Unknowns
 ○ Standards



PCR Standard Curve: Data 27-Jan-03 1233ileff.opd

Determination of the qPCR reaction efficiency


4 methods for determining **E** of the qPCR:

1. Calculated from the slope of the standard (calibration) curve
- often E overestimated


Possible for each individual reaction:

2. Calculated from fluorescence growth history using linear regression - "manual" method - often E underestimated
3. Fitting the curve according to the assumed model to the fluorescence values from the 1st to the last cycle - often E underestimated
4. Calculated from polynomial curve fitting to fluorescence data from phase 2 only - intermediate values


M. W. Pfaffl: *Quantification strategies in real-time PCR* in *A-Z of quantitative PCR* (Editor: S.A. Bustin)



Determination of the qPCR reaction efficiency based on standard curves

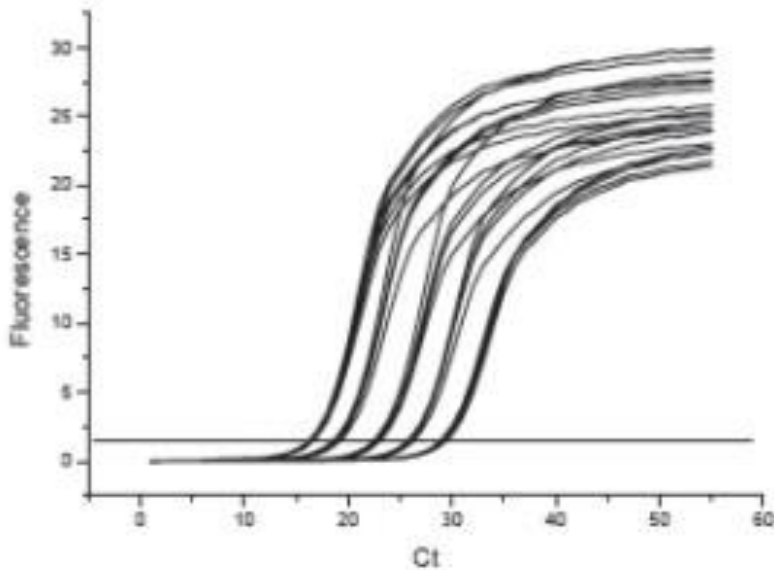


**Serial dilutions,
min. 5, better 6 to 8**

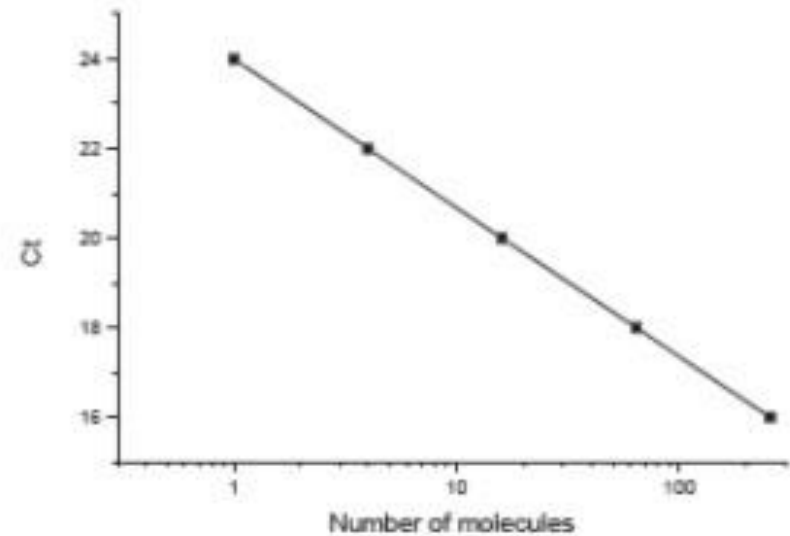

$$E = 10^{-1/\text{slope} - 1}$$

TATA Biocenter



qPCR reaction equation


$$N_{Ct} = N_0 (1 + E)^{Ct}$$

N_{Ct} : number of molecules after **Ct** cycles of amplification

N_0 : initial number of molecules

E : PCR reaction efficiency

Ct : the value of the threshold cycle



The PFAFFL method or the Relative Quantification Method


Michael W. Pfaffl

„A new mathematical model for relative quantification in real-time RT-PCR“

Nucleic Acids Research, 2001, 29:2002-2007


<https://doi.org/10.1093%2Fnar%2F29.9.e45>

NORTHERN

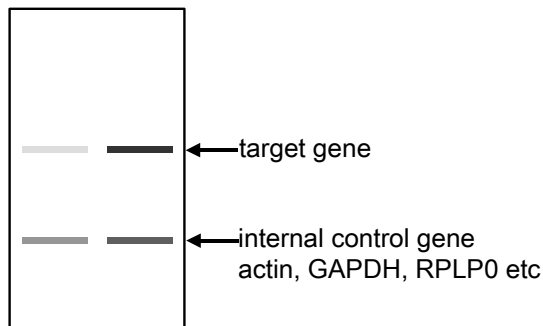

$$\text{ratio} = \frac{\text{fold increase in target gene}}{\text{fold increase in reference gene}}$$

Microbiology and Immunology On-line; University of South Carolina School of Medicine





Cursor Standard Unknown Blank + Control - Control Pu


| | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 |
|---|---|---|---|---|---|---|---|---|---|
| A | | | | | | | | | |
| B | | | | | | | | | |
| C | | C | C | C | | E | E | E | |
| D | | | | | | | | | |
| E | | | | | | | | | |
| F | | C | C | C | | E | E | E | |
| G | | | | | | | | | |

←triplicates cDNA


}target primers

←triplicates cDNA

}reference primers

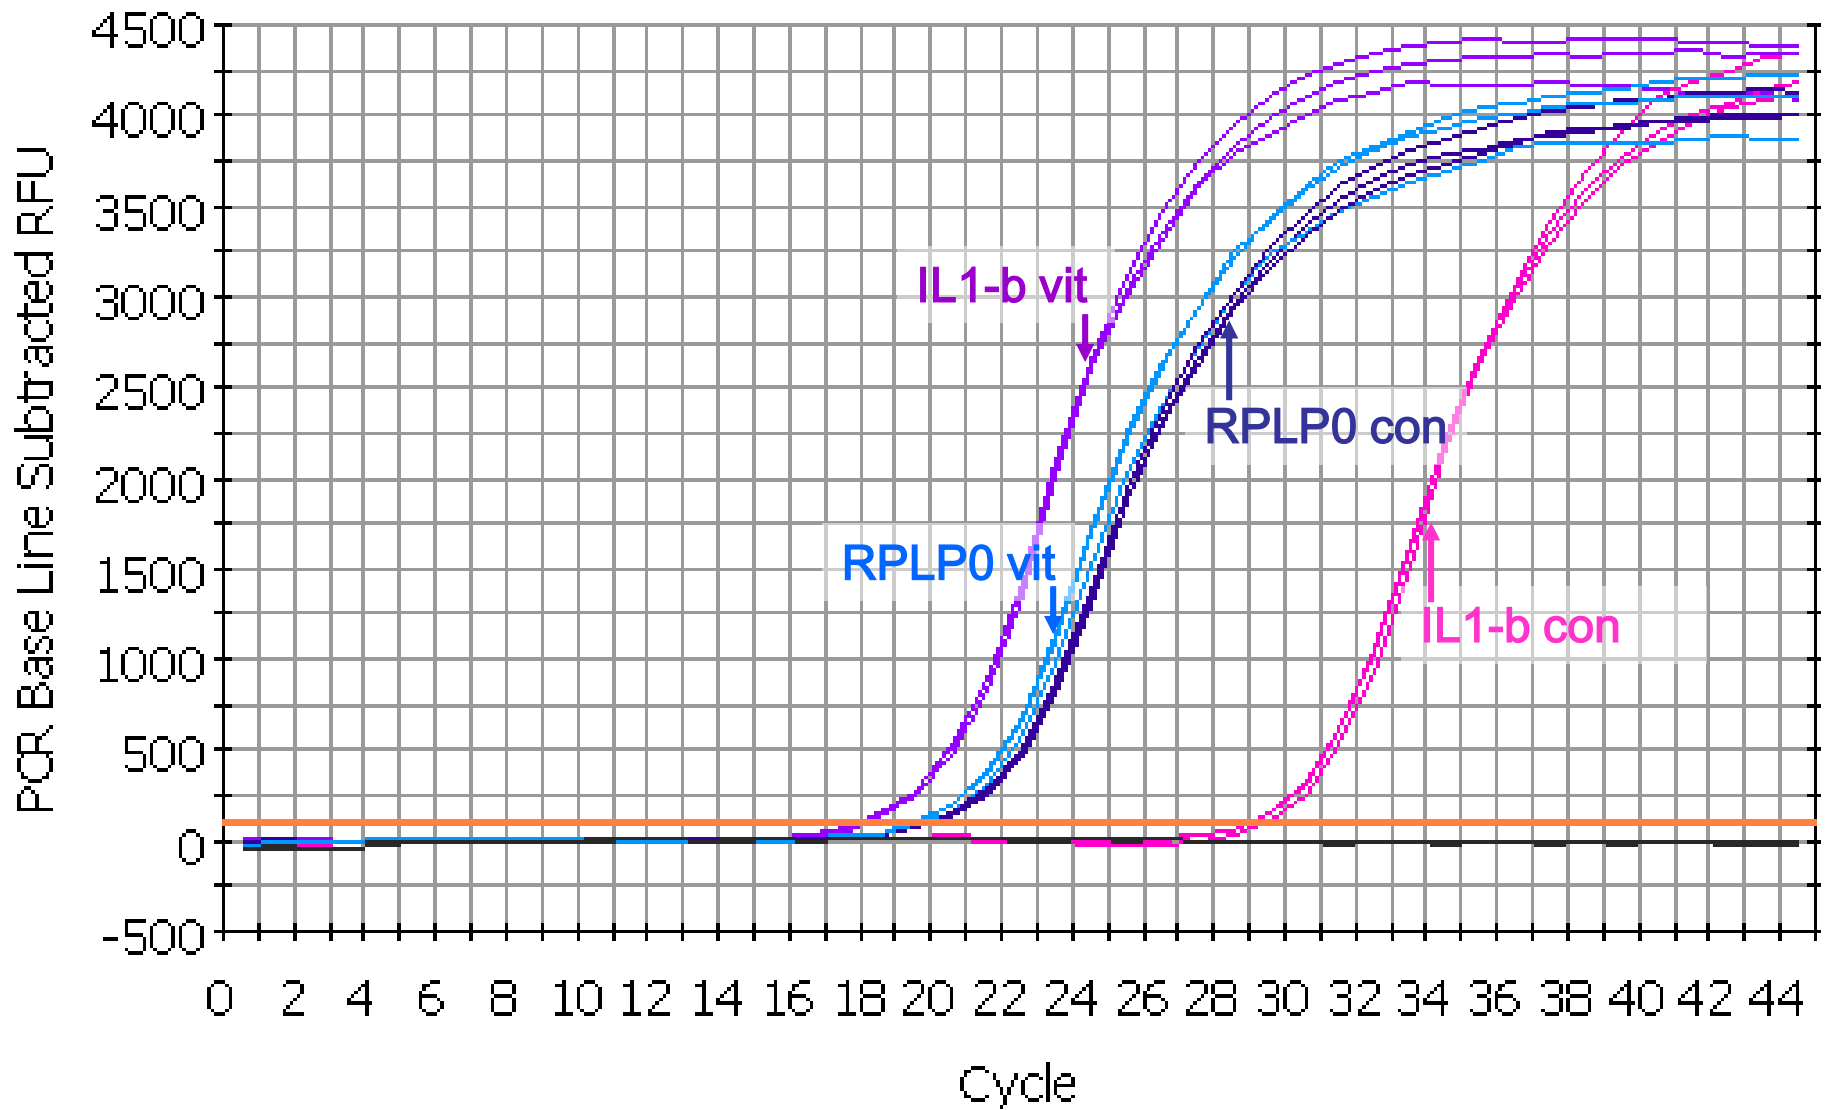


PCR Amplification vs Cycle: Data 26-Feb-03 1147.opd

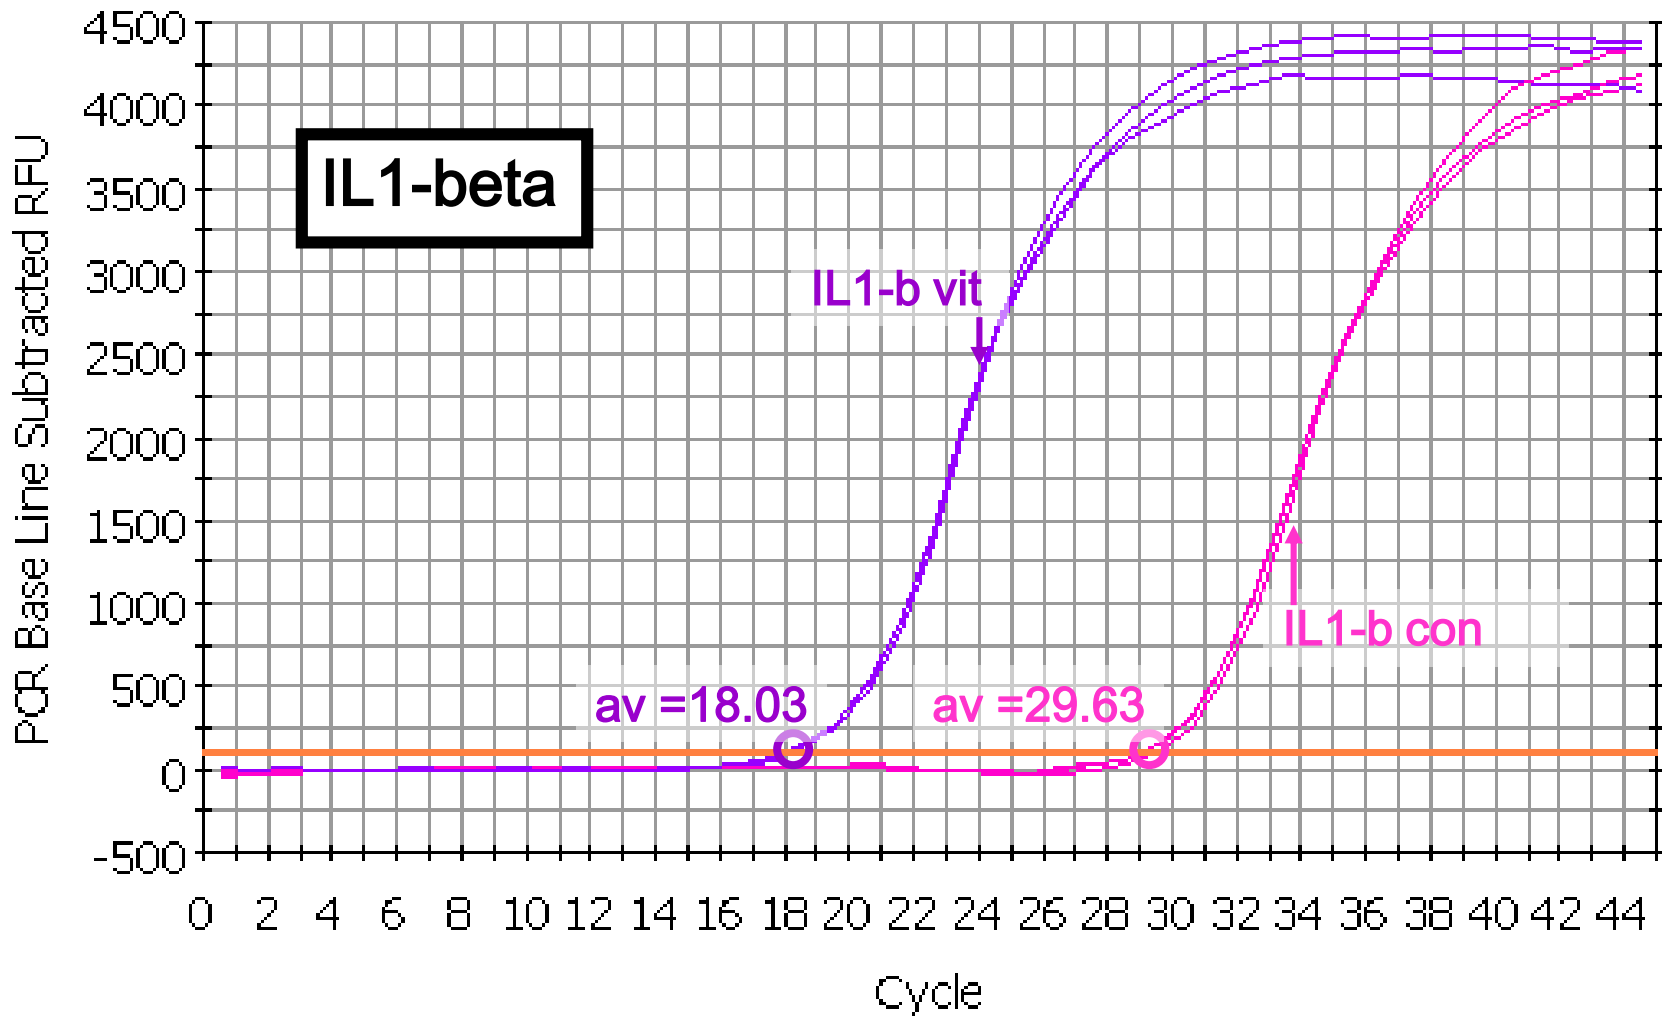



AFTER N CYCLES: change = (efficiency)ⁿ

AFTER N CYCLES: ratio vit/con = (1.93)^{29.63-18.03} = 1.93^{11.60} = 2053

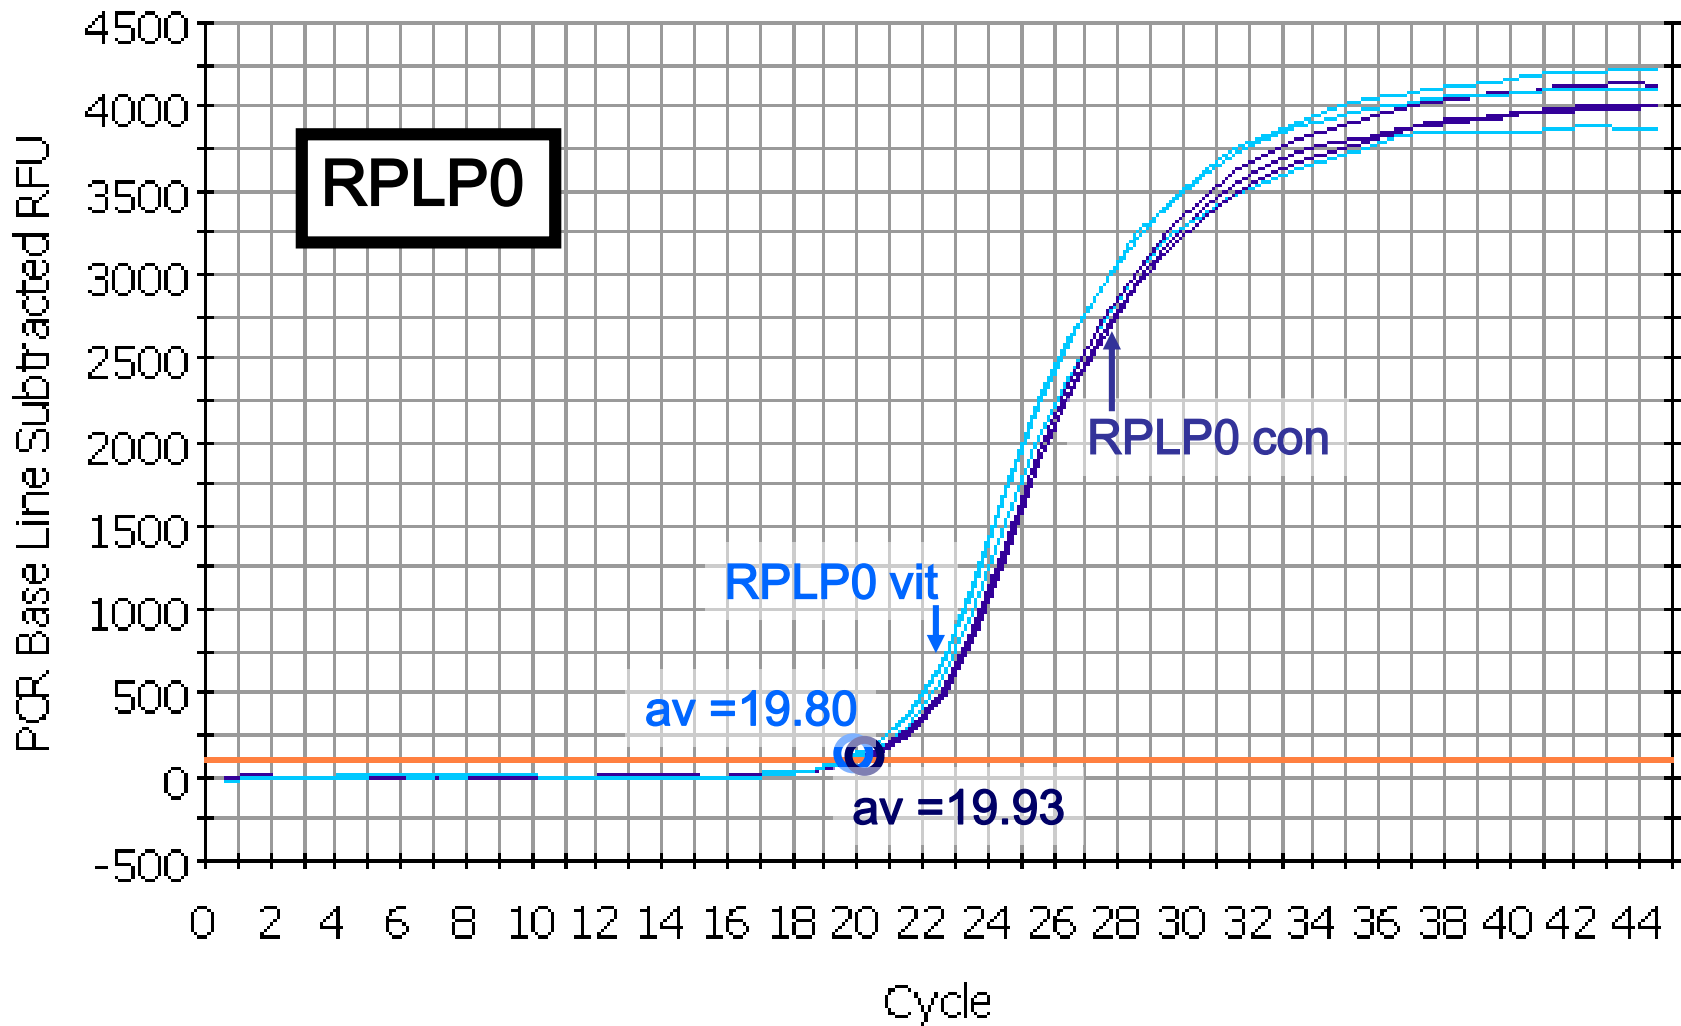

AFTER N CYCLES: change = (efficiency)ⁿ

AFTER N CYCLES: ratio vit/con = (1.87)^{19.93-19.80} = 1.87^{0.13} = 1.08

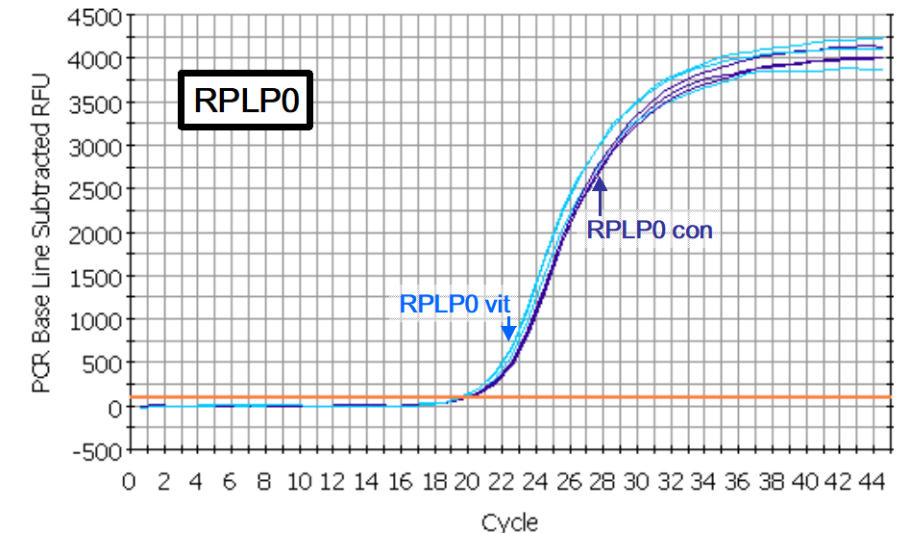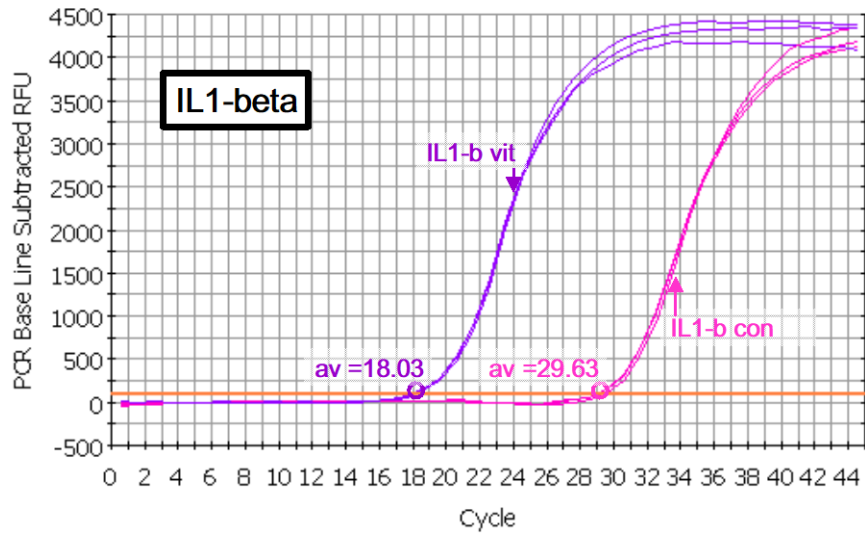

AFTER N CYCLES: increase = (efficiency)ⁿ

$$\text{Ratio vit/con} = (1.93)^{29.63-18.03} = 1.93^{11.60} = 2053$$

AFTER N CYCLES: increase = (efficiency)ⁿ

$$\text{Ratio vit/con} = (1.87)^{19.93-19.80} = 1.87^{0.13} = 1.08$$

$$\text{ratio} = \frac{\text{change in IL1-B}}{\text{change in RPLP0}} = \frac{2053}{1.08} = 1901$$

$$\text{ratio} = \frac{(E_{\text{target}})^{\Delta \text{Ct target (control-treated)}}}{(E_{\text{ref}})^{\Delta \text{Ct ref (control-treated)}}$$

Determination of reaction efficiency is essential!

Given: slope: -3.9 from a standard curve

Ct(sample A) = 23.5

Ct(sample B) = 26.5

Calculate: (A) PCR efficiency


$$E = 10^{-1/\text{slope}} - 1 = 80 \%$$

(B) Relative expression between sample A and B:

$$(1+E)^{\Delta C_t} = 1.80^{(26.5-23.5)} = 5.8$$

(C) Interpretation:

Sample A contains 5.8 times more target than sample B



Determination of reaction efficiency is essential!

Given: slope: -3.5 from a standard curve

$$Ct(\text{sample A}) = 23.5$$

$$Ct(\text{sample B}) = 26.5$$


Calculate the relative expression:

$$E = 10^{-1/\text{slope}} - 1 = 93\%$$

$$(1+E)^{\Delta Ct} = 1.93^{(26.5-23.5)} = 7.2$$


Interpretation:

The relative expression increased from 5.8 to 7.2 when the PCR efficiency was 13% higher.






Determination of reaction efficiency is essential!

| <u>E = 80 %</u> | <u>Ct_A = 20</u> | <u>E = 95%</u> |
|-----------------|----------------------------|----------------|
| 1.8 | Ct _B = 21 | 1.95 |
| 5.8 | Ct _B = 23 | 7.4 |
| 19 | Ct _B = 25 | 28 |
| 61 | Ct _B = 27 | 107 |
| 198 | Ct _B = 29 | 408 |



Error in qPCR reaction accumulates exponentially!

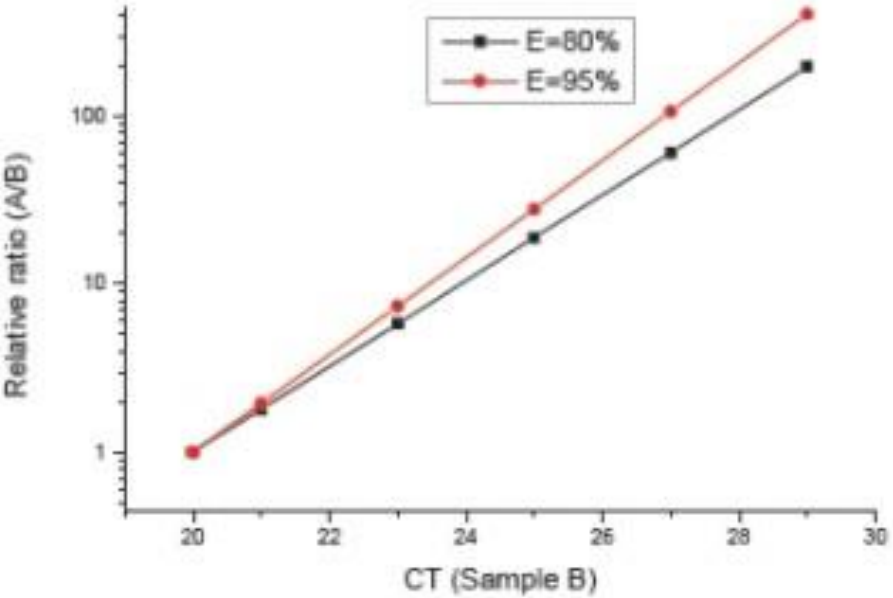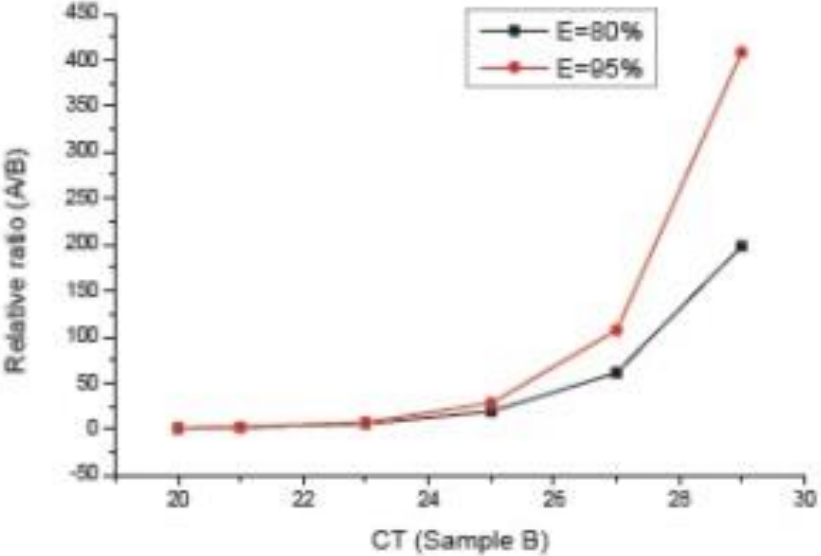


The mRNA equation

$$\frac{N_A}{N_B} = K_{RS} \frac{\eta_B (1 + E_B)^{CT_B - 1}}{\eta_A (1 + E_A)^{CT_A - 1}}$$

η - RT efficiency CT - value (cycle) Ct


E - PCR yield K_{RS} - relative qPCR sensitivity



Quantification: 2 samples, 2 genes

$$\frac{\text{Sample A}}{\text{Sample B}} = \frac{\left[\frac{N_{0_{tar}}}{N_{0_{ref}}} \right]_{\text{Sample A}}}{\left[\frac{N_{0_{tar}}}{N_{0_{ref}}} \right]_{\text{Sample B}}} = \frac{\left[\frac{(1 + E_{ref})^{Ct_{ref}}}{(1 + E_{tar})^{Ct_{tar}}} \right]_{\text{Sample A}}}{\left[\frac{(1 + E_{ref})^{Ct_{ref}}}{(1 + E_{tar})^{Ct_{tar}}} \right]_{\text{Sample B}}}$$


$$\frac{\text{Sample A}}{\text{Sample B}} = \frac{(1 + E_{ref})^{CtA_{ref} - CtB_{ref}}}{(1 + E_{tar})^{CtA_{tar} - CtB_{tar}}}$$




"garbage in, garbage out"

"Real-time quantitative RT-PCR is a wonderful method for fast, accurate, sensitive and cost-effective gene expression analysis. However, the simplicity of the technology itself makes it vulnerable for **abuse in experiments** in which the operator **does not perform the required quality control throughout the entire procedure.**"

Derveaux S. et al, Methods 50 (2010) 227-230




RT-qPCR in practice



RNA quality is a key factor!!!

DNase treatment
1h, 37° C

- +

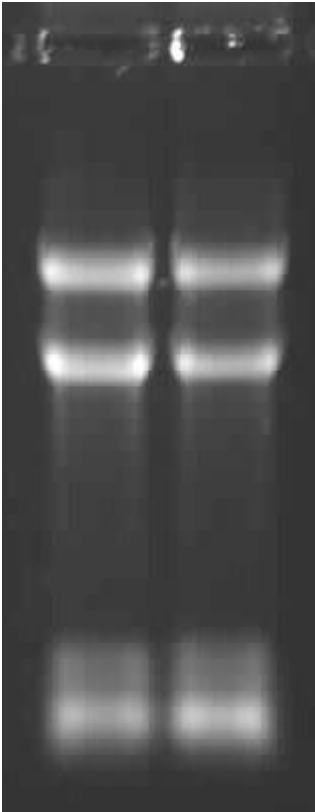

RNA quality = **purity + integrity**

Purity – determined spectrophotometrically


($OD_{260/230} > 2.0$; $OD_{260/280} > 1.8$)

RNA quality control after isolation is always necessary!

DNase treatment is always necessary!


20% of human genes have 1 exon, or there are expressed retropseudogenes or copies lacking introns!!!

Recommended use of RNase inhibitors at RT!




RNA quality assays

5'-3' RNA ends integrity test

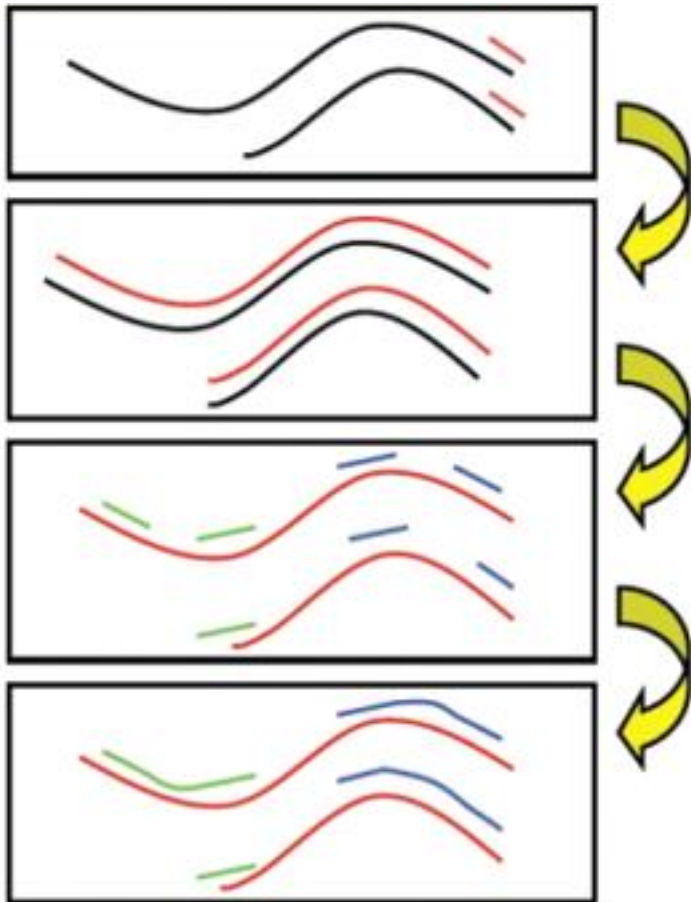


Microfluidic Analyzers

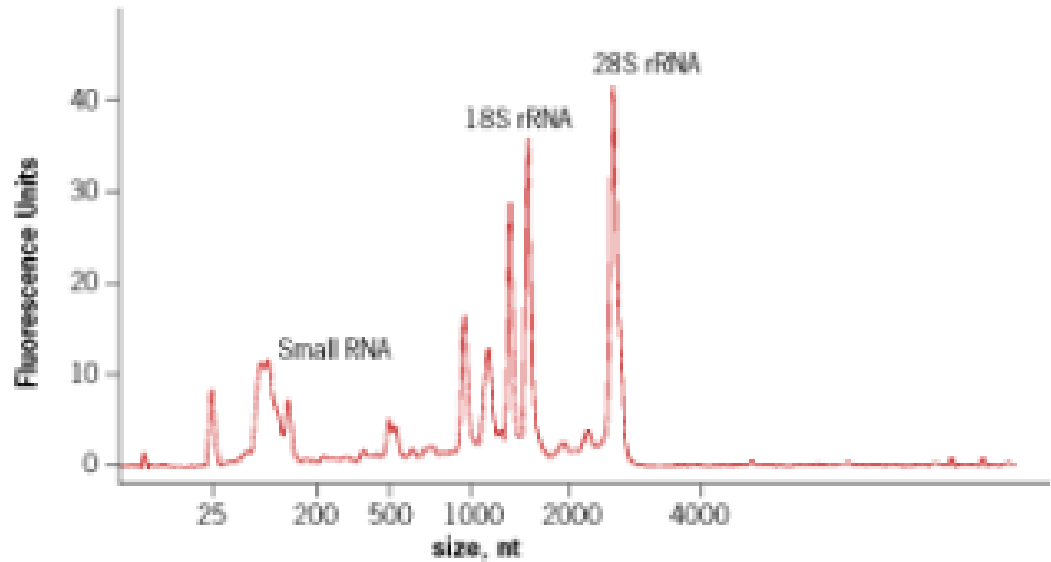


- **Agilent: Bioanalyzer, Tapestation**
- **Biorad: Experion**
- **Capillary electrophoresis**

Quality affects results!!!


RIN: "RNA Integrity Number", min. 7
(according to Bioanalyzer, Agilent Technologies).

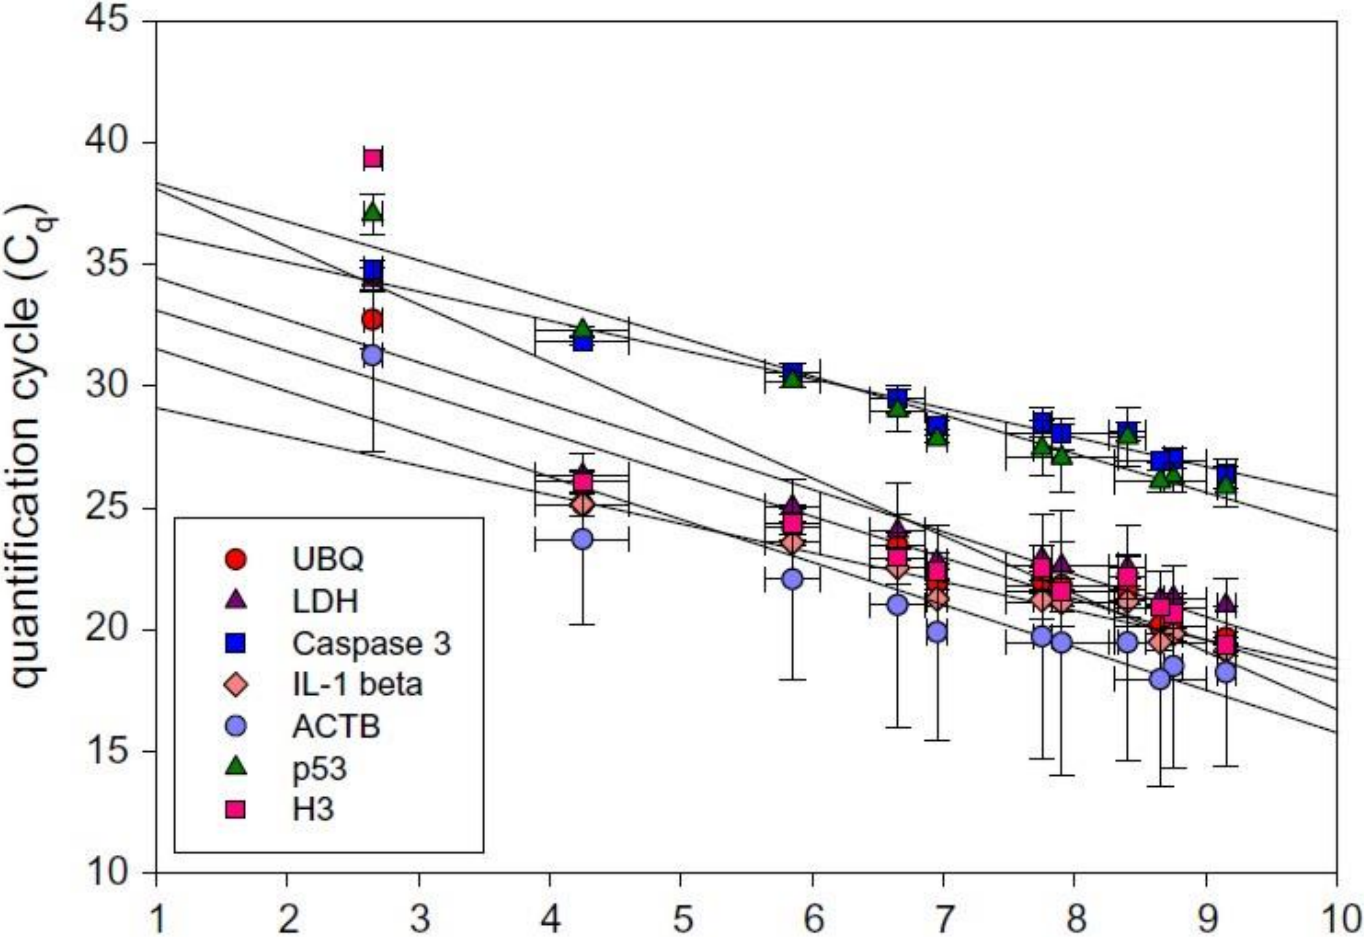

Primer design strategies to minimize signals for gDNA contamination

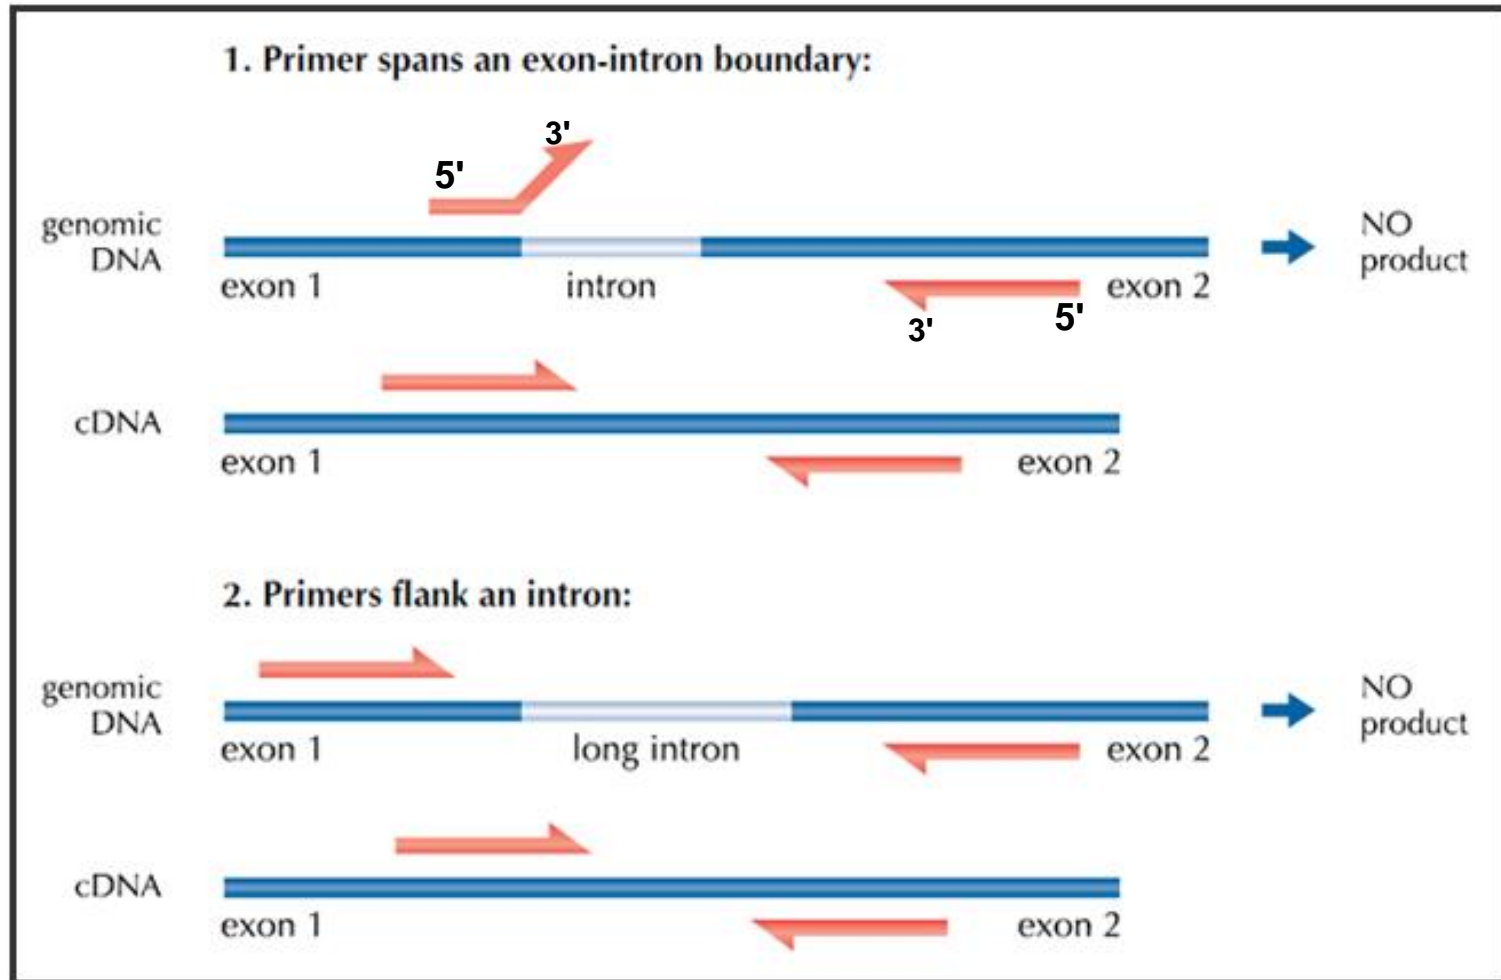


<https://www.thermofisher.com/pl/en/home/brands/thermo-scientific/molecular-biology/molecular-biology-learning-center/molecular-biology-resource-library/basic-principles-rt-qpcr.html>



**The most crucial step
of RT-qPCR is the**

**reverse transcription
reaction!!!**



Efficiency and specificity of RT

Efficiency and specificity of reverse transcription reaction **STRONGLY** depends on:

- **Methods of priming**
- **Type of reverse transcriptase (features of the enzyme)**
- **The sequence of a particular RNA molecule – it's tendency to form complex secondary structures**
- **Efficiency differences can be as high as 100X!!!**
- **The optimal RT conditions should always be determined experimentally**

RT priming methods


– advantages and disadvantages

| | Primer Options | Structure and Function | Advantages | Disadvantages |
|------------------------------|-------------------------------------|--|--|---|
| <p>Standard oligo dT</p> | Oligo(dT)s (or anchored oligo(dT)s) | Stretch of thymine residues that anneal to poly(A) tail of mRNA; anchored oligo(dT)s contain one G, C, or A (the anchor) residue at the 3' end | <ul style="list-style-type: none"> •Generation of full length cDNA from poly(A)-tailed mRNA •Good to use if little starting material is available •Anchor ensures that the oligo(dT) primer binds at the 5' end of the poly(A) tail of mRNA | <ul style="list-style-type: none"> •Only amplify gene with a poly(A) tail •Truncated cDNA from priming internal poly(A) sites*2 •Bias towards 3' end* *Minimized if anchored oligo(dT)s are used. |
| <p>Anchored oligo dT</p> | | | | |
| <p>Random primers</p> | Sequence Specific Primers | Custom made primers that target specific mRNA sequence | <ul style="list-style-type: none"> •Specific cDNA pool •Increased sensitivity •Use reverse qPCR primer | <ul style="list-style-type: none"> •Synthesis is limited to one gene of interest |
| <p>Gene-specific primers</p> | | | | |

<https://www.thermofisher.com/pl/en/home/brands/thermo-scientific/molecular-biology/molecular-biology-learning-center/molecular-biology-resource-library/basic-principles-rt-qpcr.html>

Effect of the priming method on RT efficiency

RT efficiency

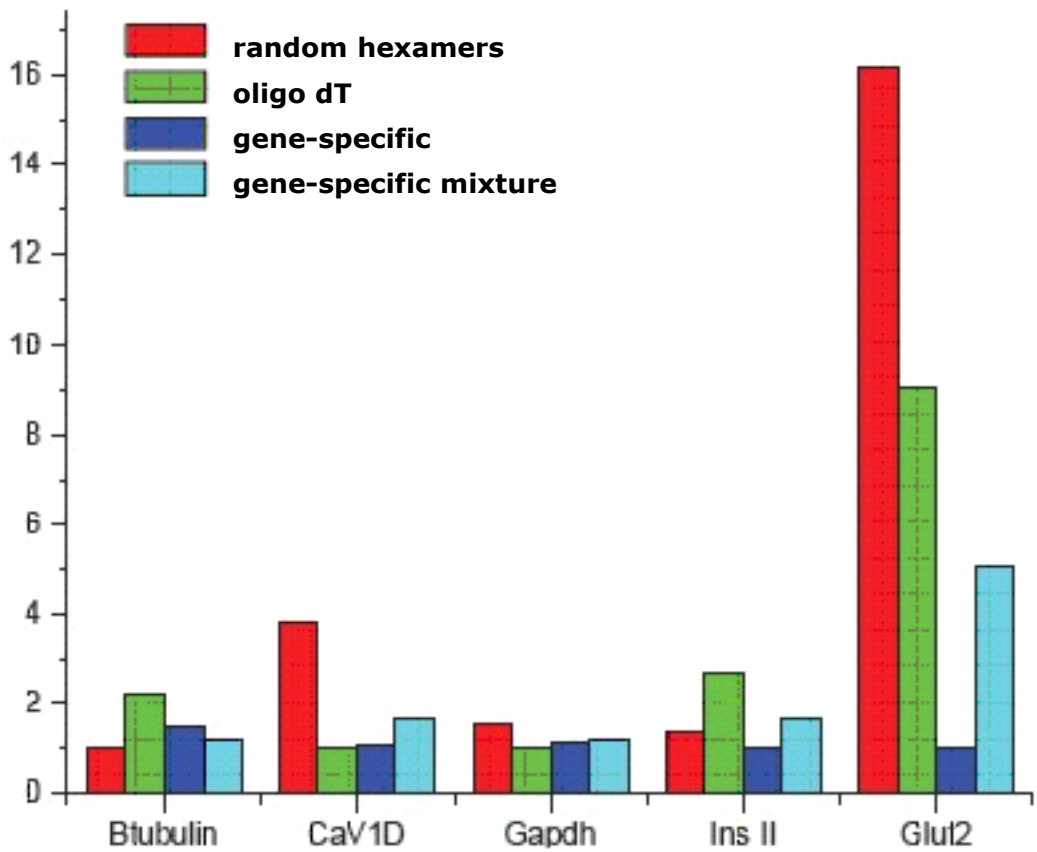

Sthalberg et al, 2004, Comparison of reverse transcriptases In gene expression analysis, Clin Chem. 50(9):1678-80.

Specificity of priming methods

| RT priming ^a | β -tubulin ^b | CaV1D ^b | GAPDH ^b | Insulin II ^b | Glut2 ^b |
|------------------------------|-------------------------------|--------------------|--------------------|-------------------------|--------------------|
| hexamers | 19.5 | <u>26.5</u> | <u>15.8</u> | 16.9 | <u>27.5</u> |
| oligo(dT) | <u>18.1</u> | 28.8 | 16.6 | <u>15.9</u> | 28.4 |
| specific | 18.8 | 28.7 | 16.4 | 17.4 | 31.8 |
| mix | 19.1 | 27.9 | 16.2 | 16.6 | 29.3 |
| max Δ Ct ^c | 1.4 | 2.3 | 0.8 | 1.5 | 4.4 |




Stahlberg et al, 2004, Comparison of reverse transcriptases
In gene expression analysis, Clin Chem. 50(9):1678-80.

Effect of the priming method on RT efficiency

| RT priming | β -tubulin ^a | CaV1D ^a | GAPDH ^a | Insulin II ^a | Glut2 ^a |
|-----------------------------------|-------------------------------|--------------------|--------------------|-------------------------|--------------------|
| <u>β-tubulin</u> | <u>18.8</u> | 28.7 | 19.0 | 18.8 | 30.6 |
| CaV1D | 27.0 | <u>28.7</u> | 19.9 | 22.8 | <i>b</i> |
| GAPDH | 23.4 | 30.1 | <u>16.4</u> | 20.1 | <u>29.7</u> |
| Insulin2 | 23.5 | 31.6 | 20.0 | <u>17.4</u> | 31.0 |
| Glut2 | 25.8 | 31.9 | 22.7 | 22.7 | 31.8 |
| <u>no primer</u> | 27.6 | 33.7 | 23.6 | 23.1 | 32.6 |


Stahlberg et al, 2004, Comparison of reverse transcriptases In gene expression analysis, Clin Chem. 50(9):1678-80.

Differences in RT reaction efficiency can reach 100X!

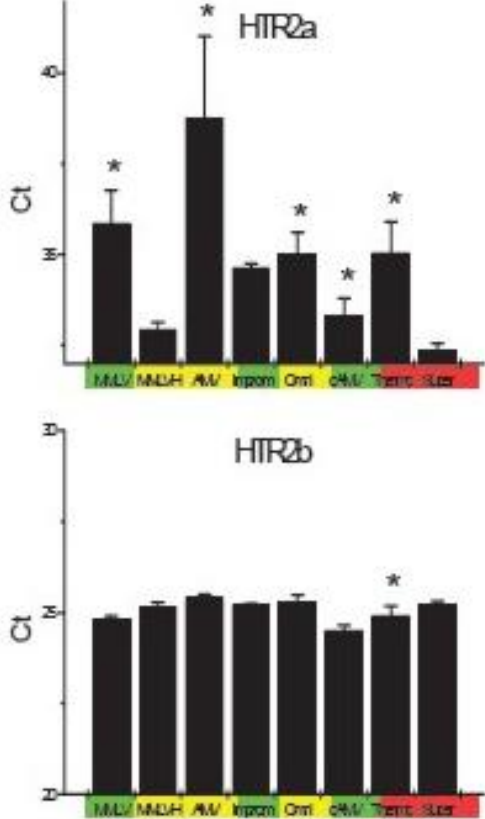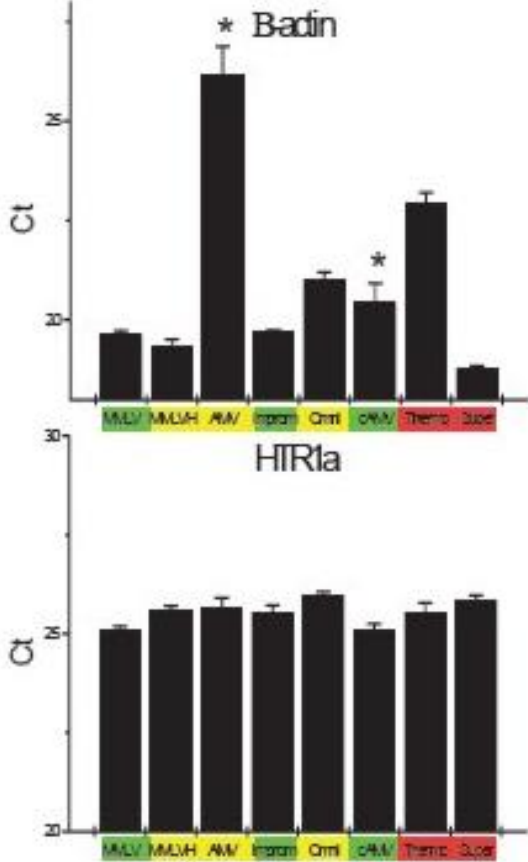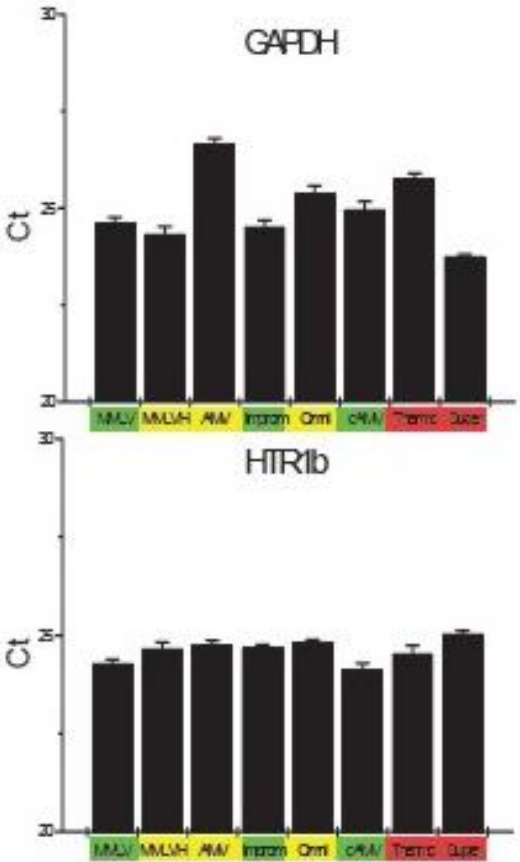

Stahlberg et al, 2004, Comparison of reverse transcriptases In gene expression analysis, Clin Chem. 50(9):1678-80.

RT optimization

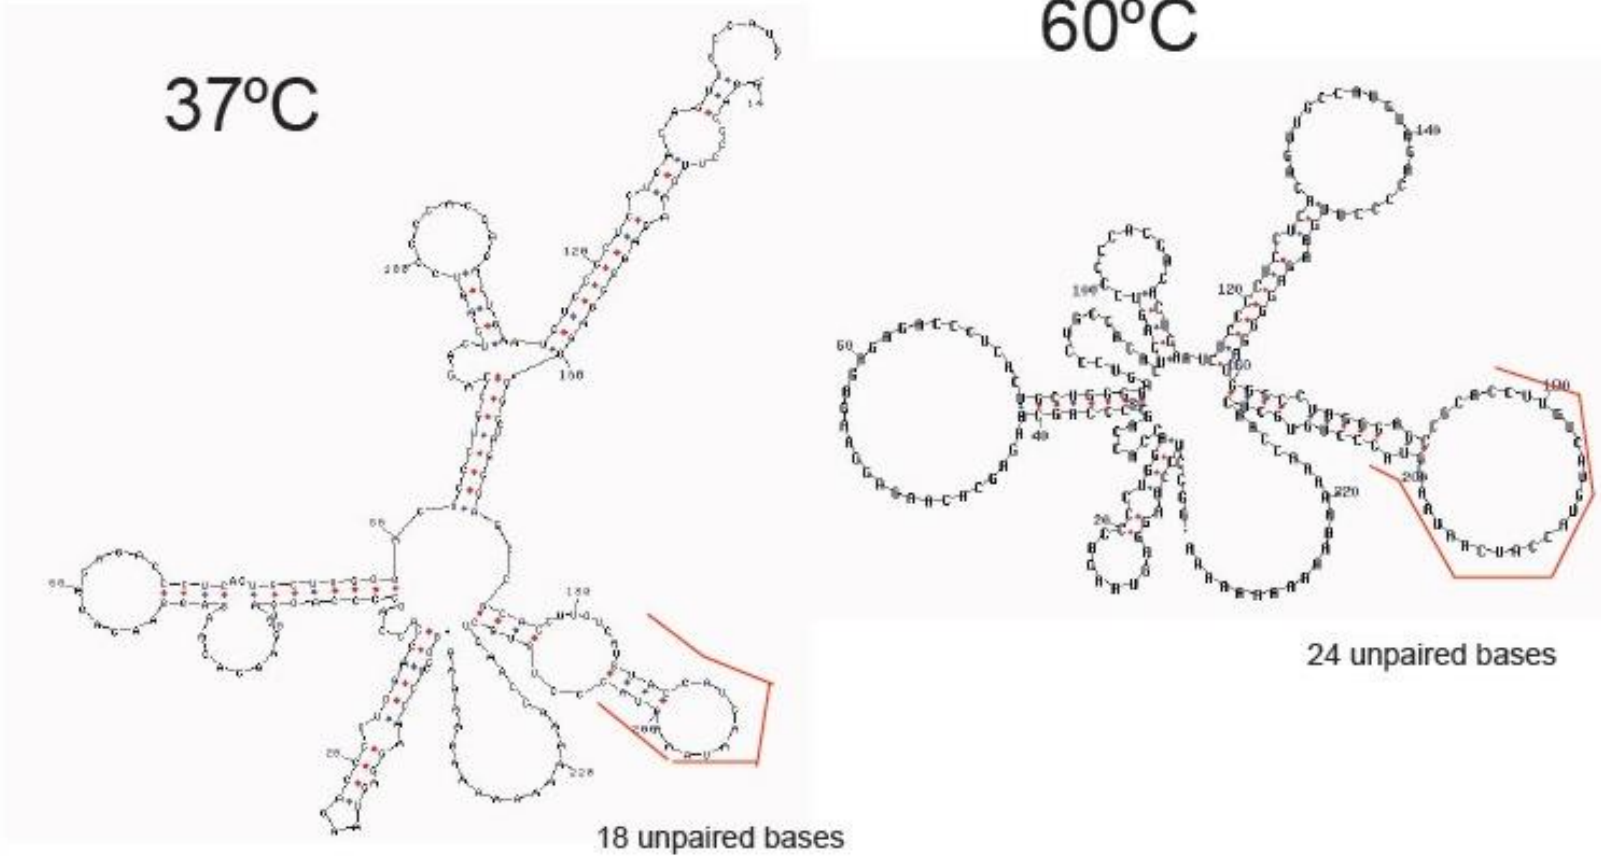

*Behind the TATA
Biocenter*


Always CONTROLS!!!

Negative Controls:


- **-RT**: control of genomic DNA contamination, necessary!
- **NTC**: "no template control": reagent purity control!!!

Positive control:

- **min. 2-3 samples**, e.g., from the standard curve - control of reaction performance! (**IRC** = inter-run calibrators)



Choice between 1-step or 2-step RT-qPCR reaction

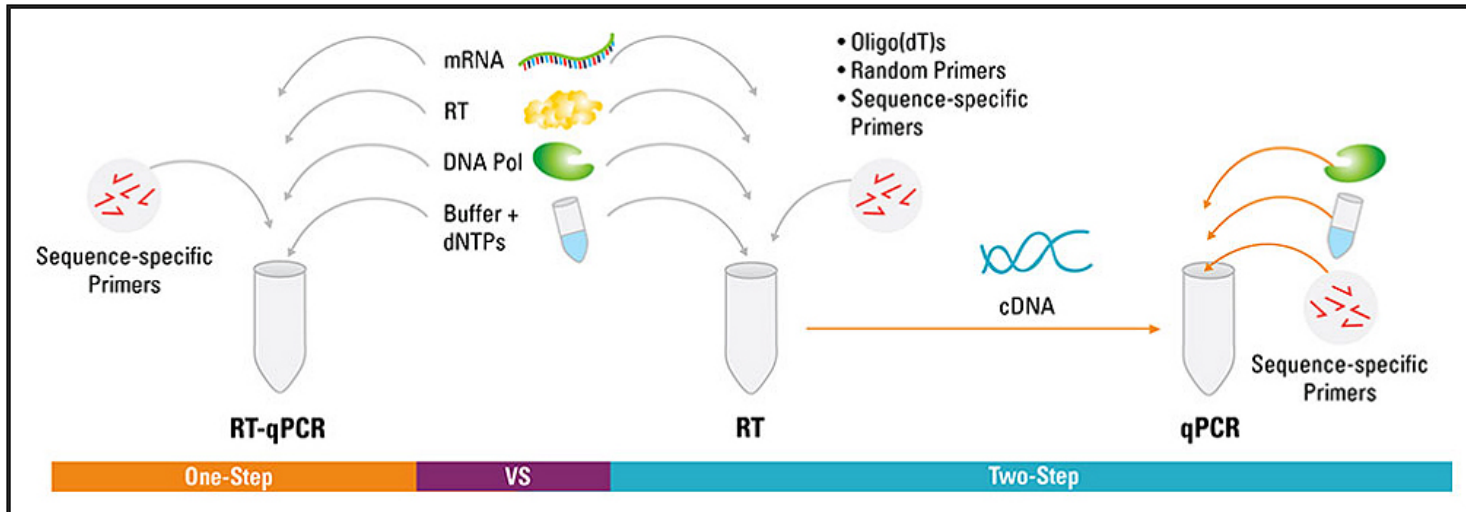

1-step


Advantages

- Less experimental variation since both reactions take place in the same tube
- Fewer pipetting steps reduces risk of contamination
- Suitable for high throughput amplification/screening Fast and highly reproducible
- A stable cDNA pool is generated that can be stored for long periods of time and used for multiple reactions
- The target and reference genes can be amplified from the same cDNA pool without multiplexing
- Optimized reaction buffers and reaction conditions can be used for each individual reaction
- Flexible priming options

2-step

Disadvantages


- Impossible to optimize the two reactions separately
- Less sensitive than two-step because the reaction conditions are a compromise between the two combined reactions
- Detection of fewer targets per sample
- The use of several tubes and pipetting steps exposes the reaction to a greater risk of DNA contamination
- Time consuming
- Requires more optimization than one-step




Good laboratory practice

IT'S BASIC!!!



- Do not pipette **less than 2 μ l** at a time by hand!
- Separate place for preparing the reaction without template and separate for adding DNA!
- **Powder-free gloves!**
- Prepare reactions in "**MIX**" not separate!
- Do not open tubes/plates after reaction in PCR rooms!
- Laminar flow chambers!





Basic analysis of qPCR reactions






Amplification curves - raw data

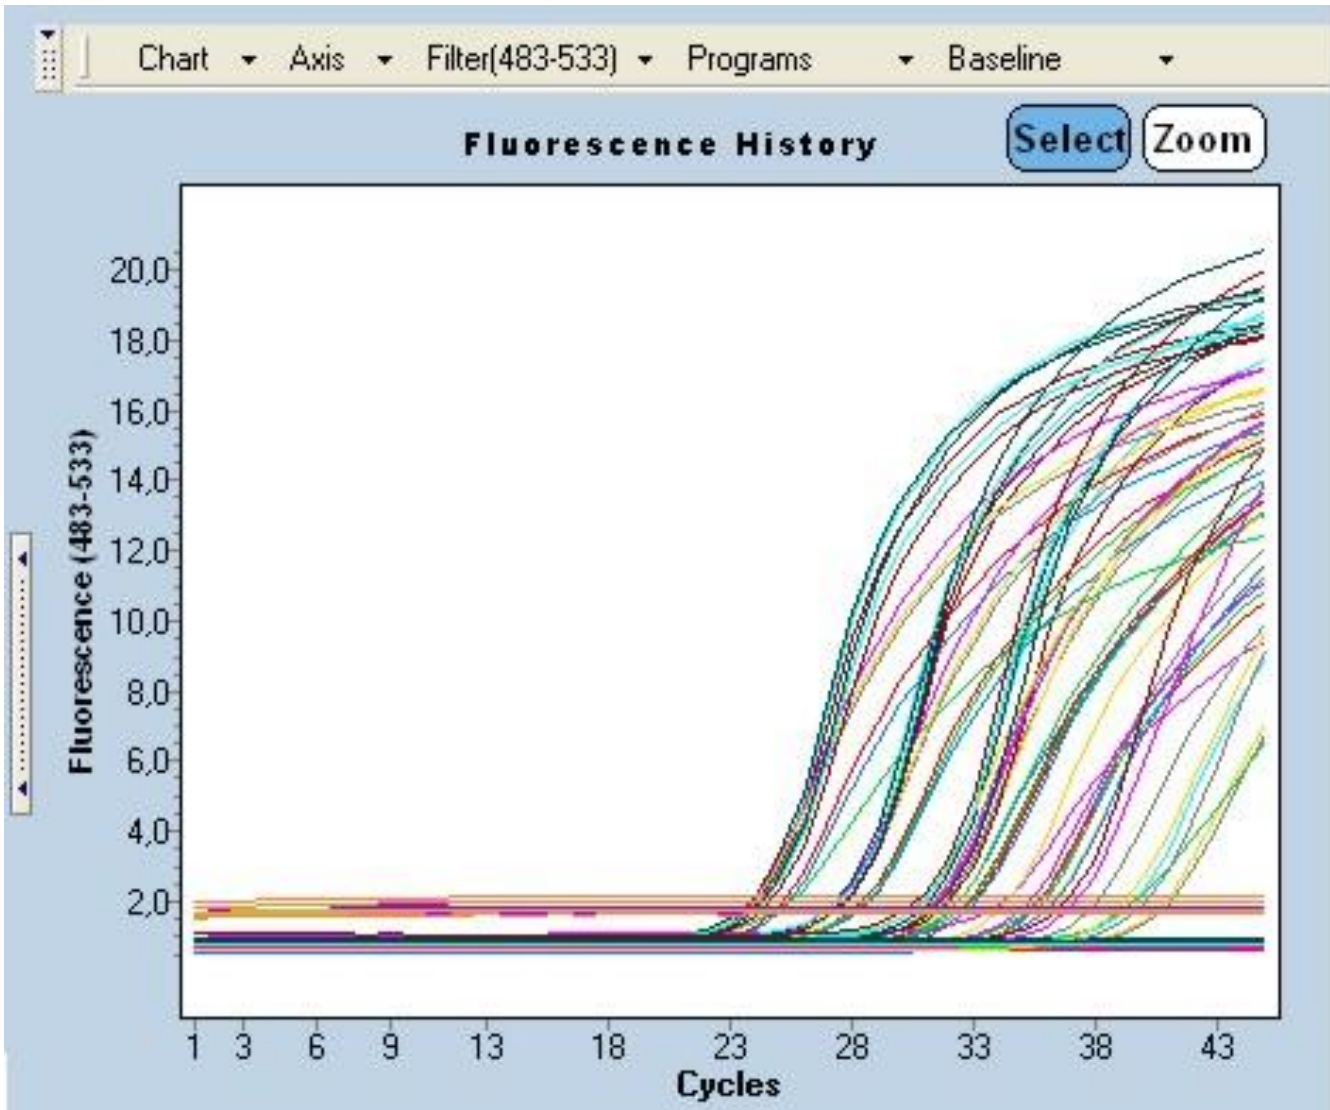

Baseline subtraction


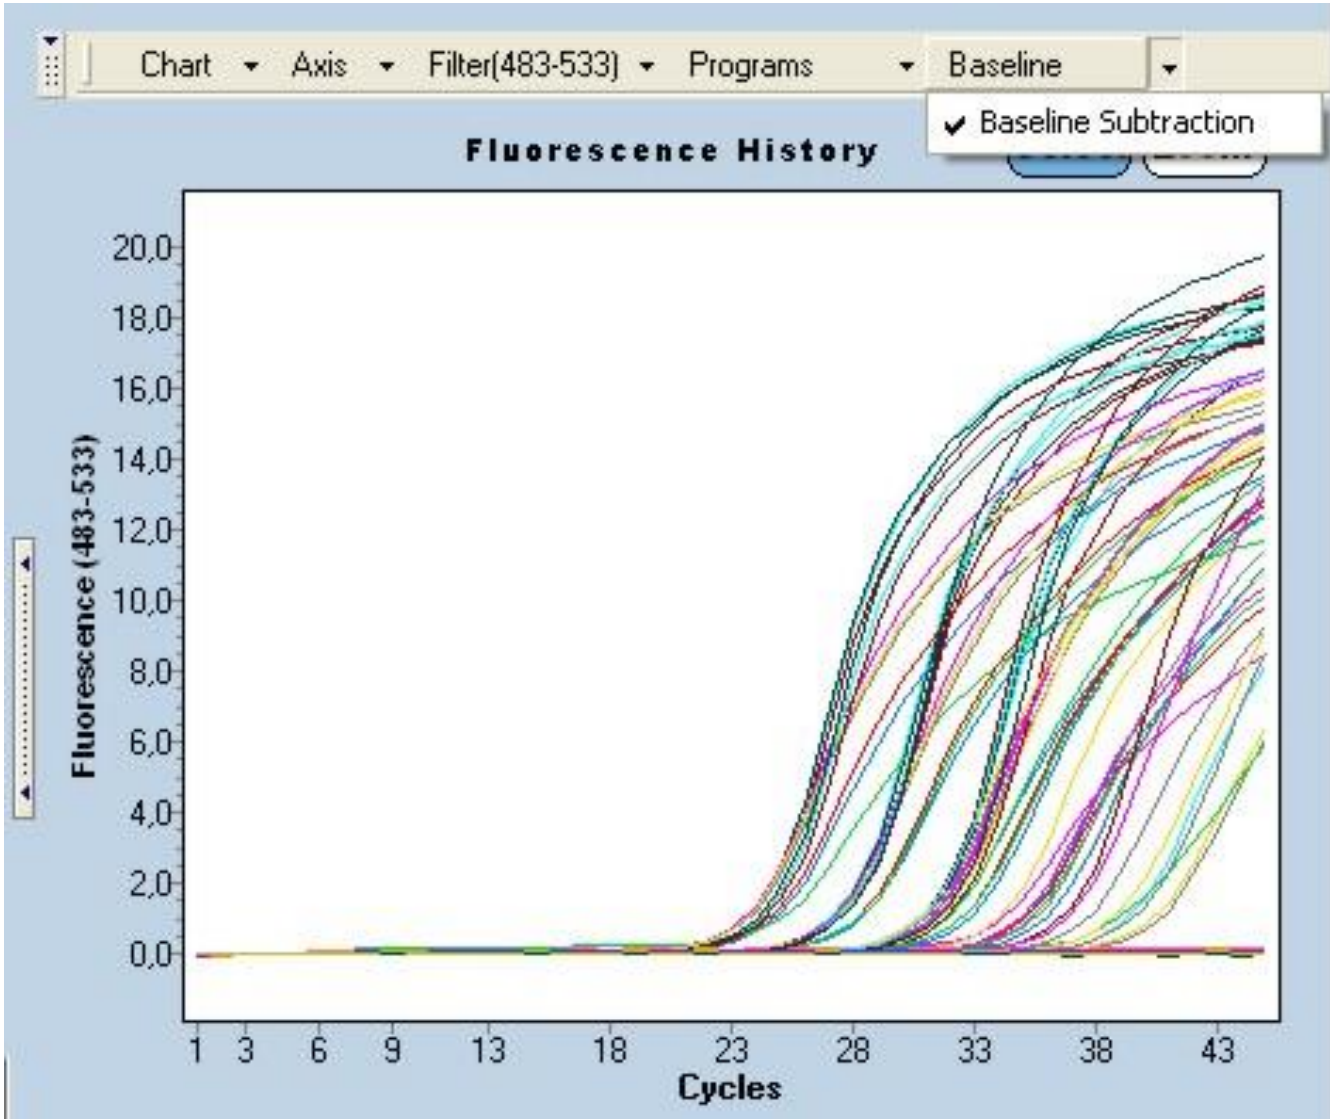


1 qPCR = 3 technical replicas!!!

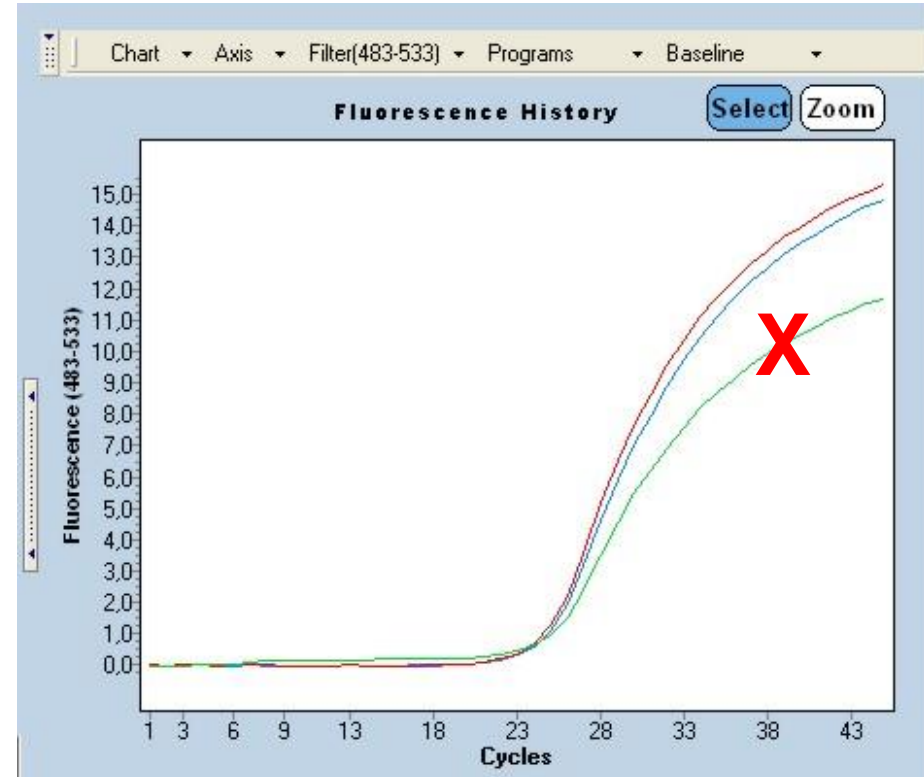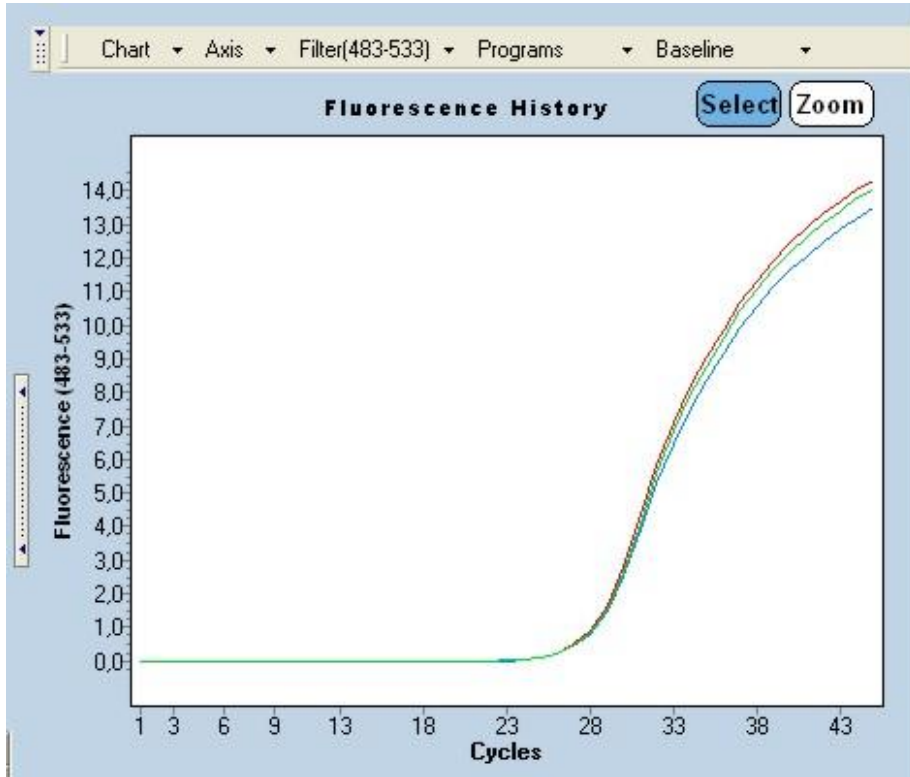



Inspection of amplification curves

Gene tested

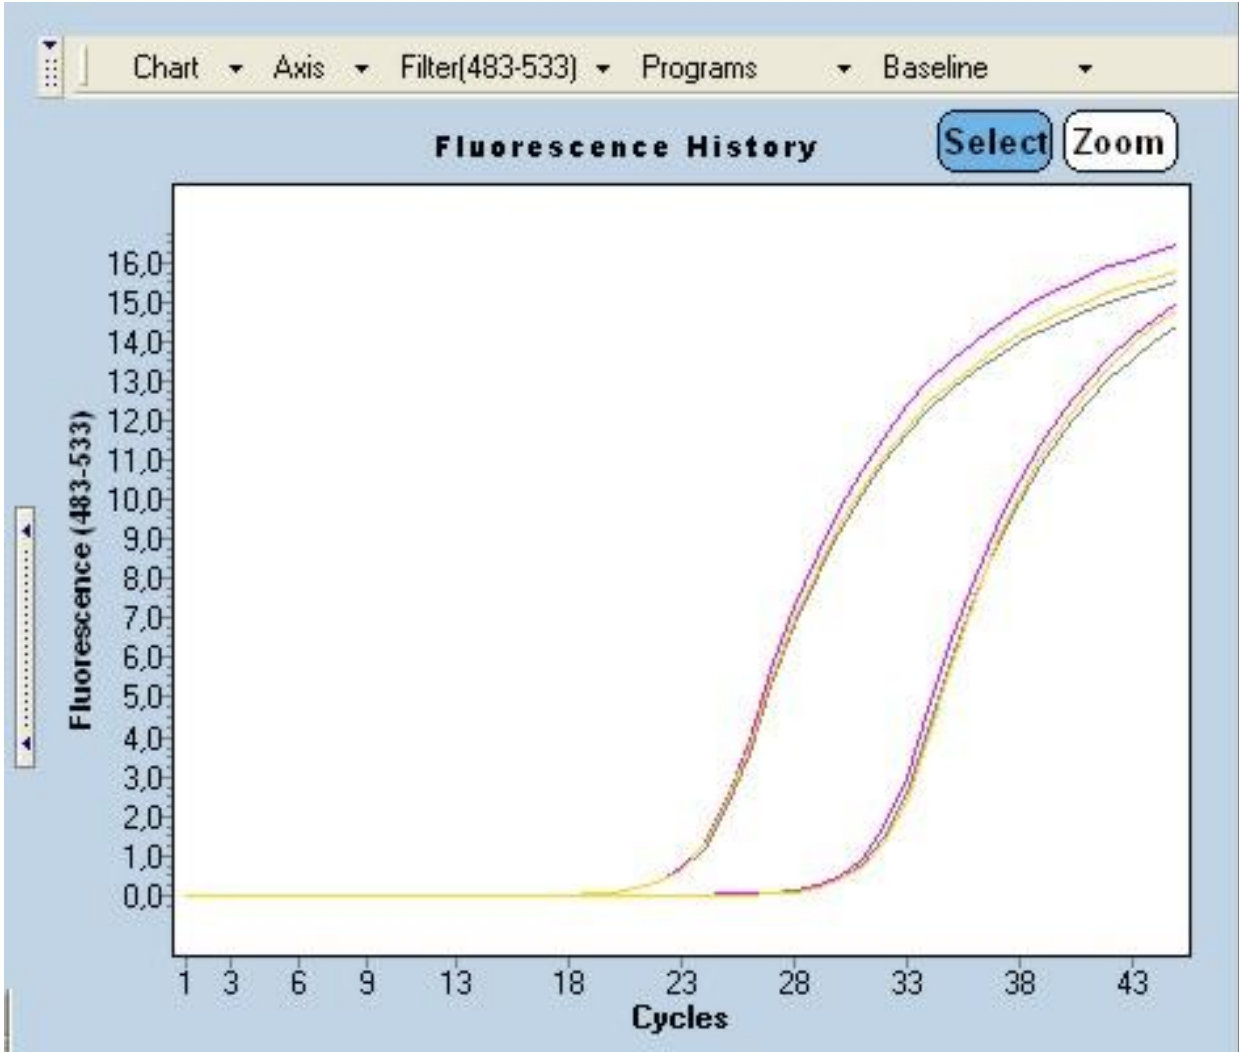



Inspection of amplification curves

Reference gene

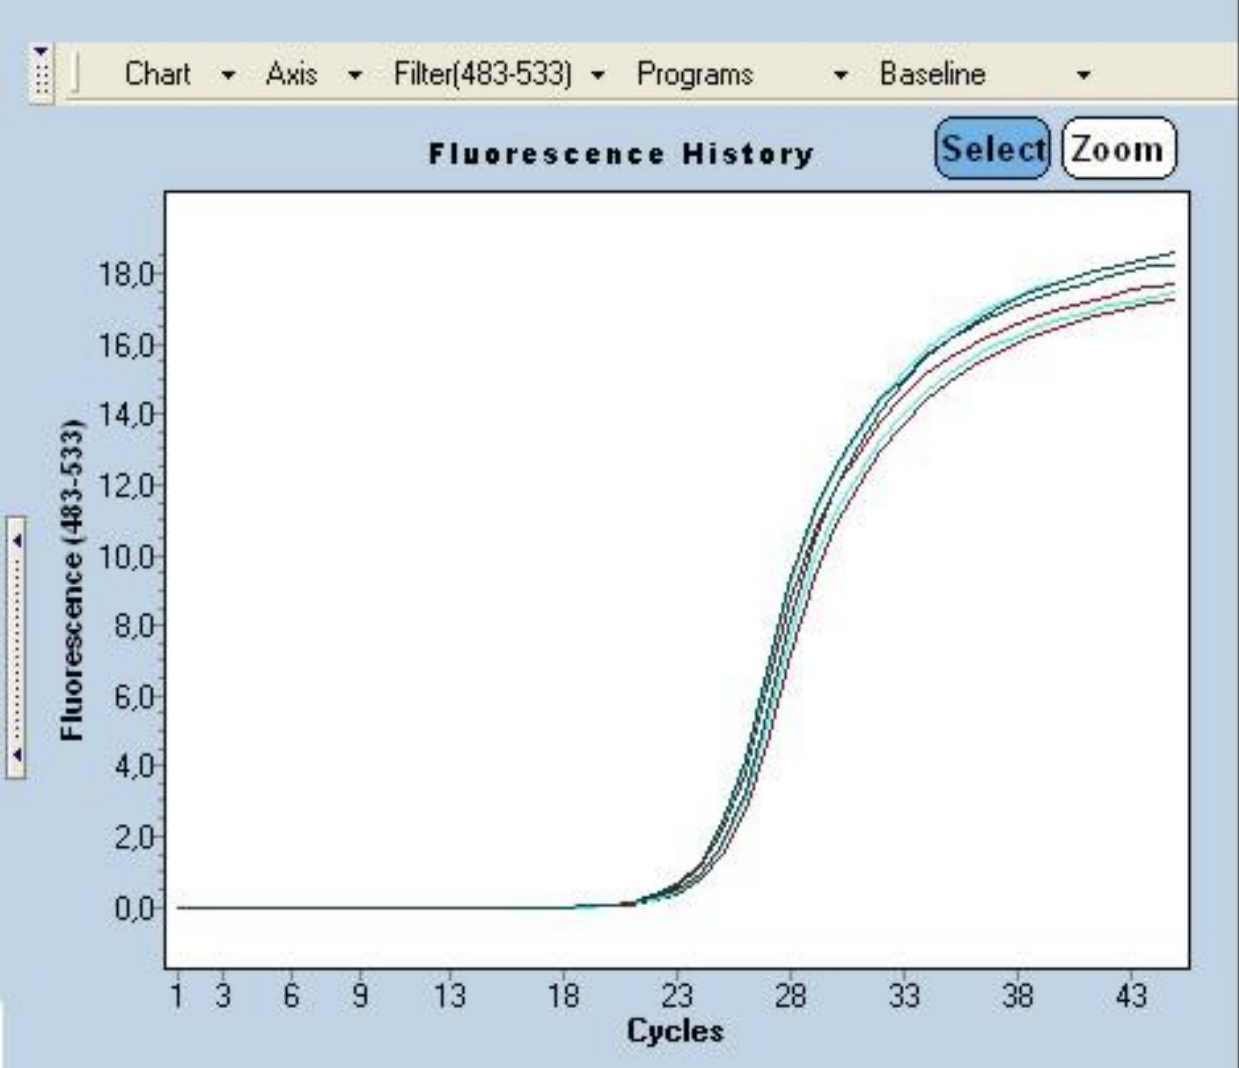



Analysis of melting curves

Possible mainly for SYBR Green

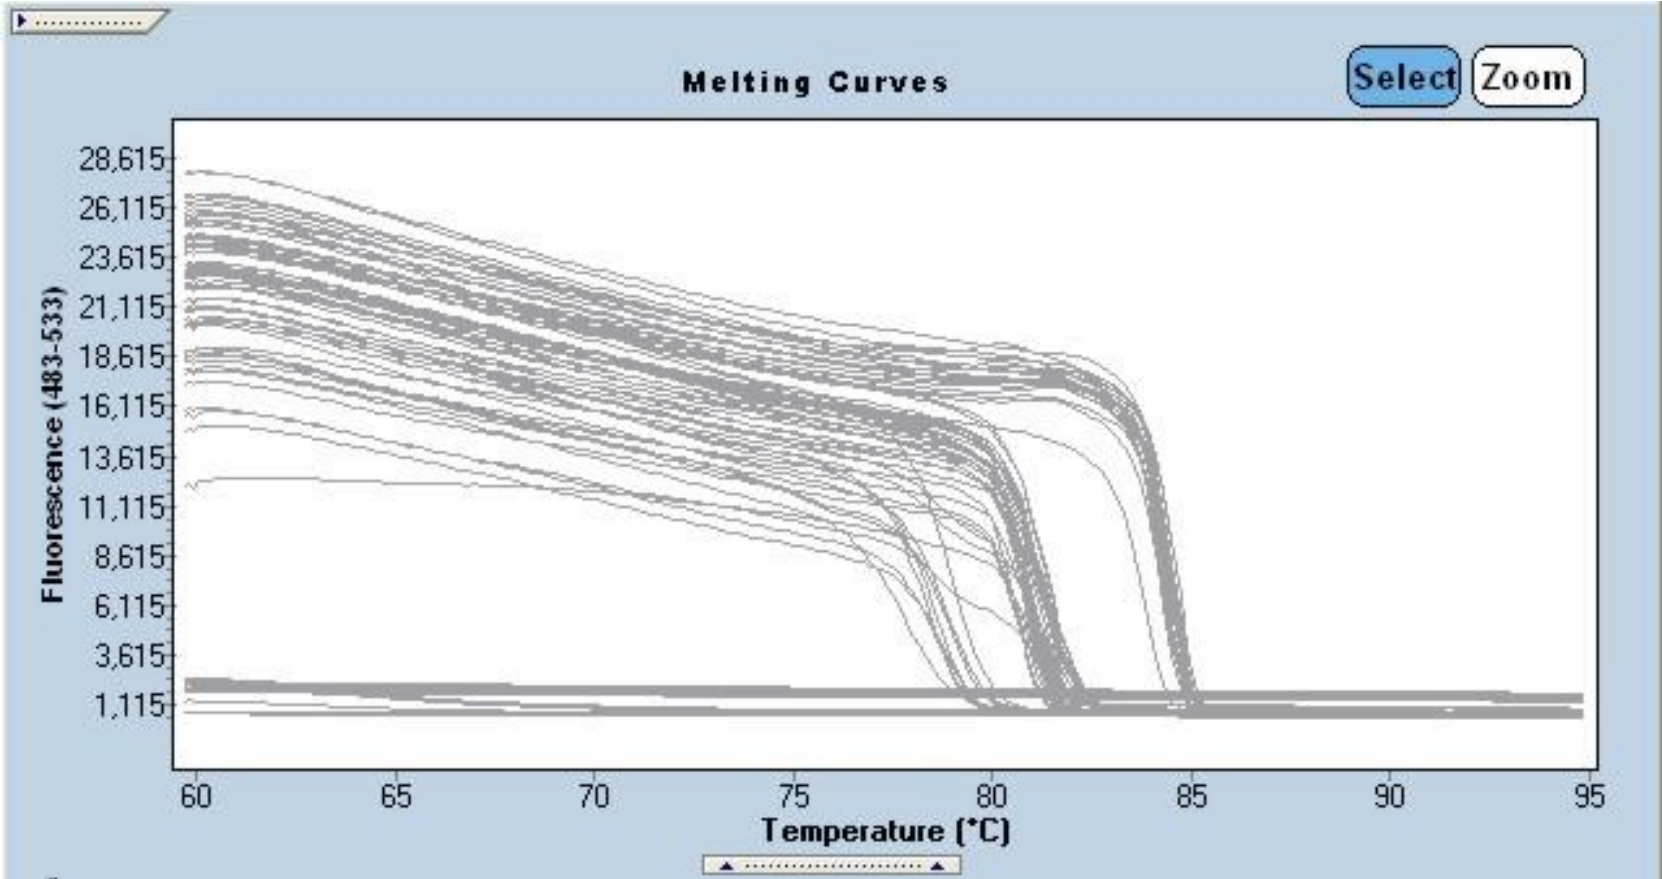



Analysis of melting curves

T_m – depends on the length and GC/AT content

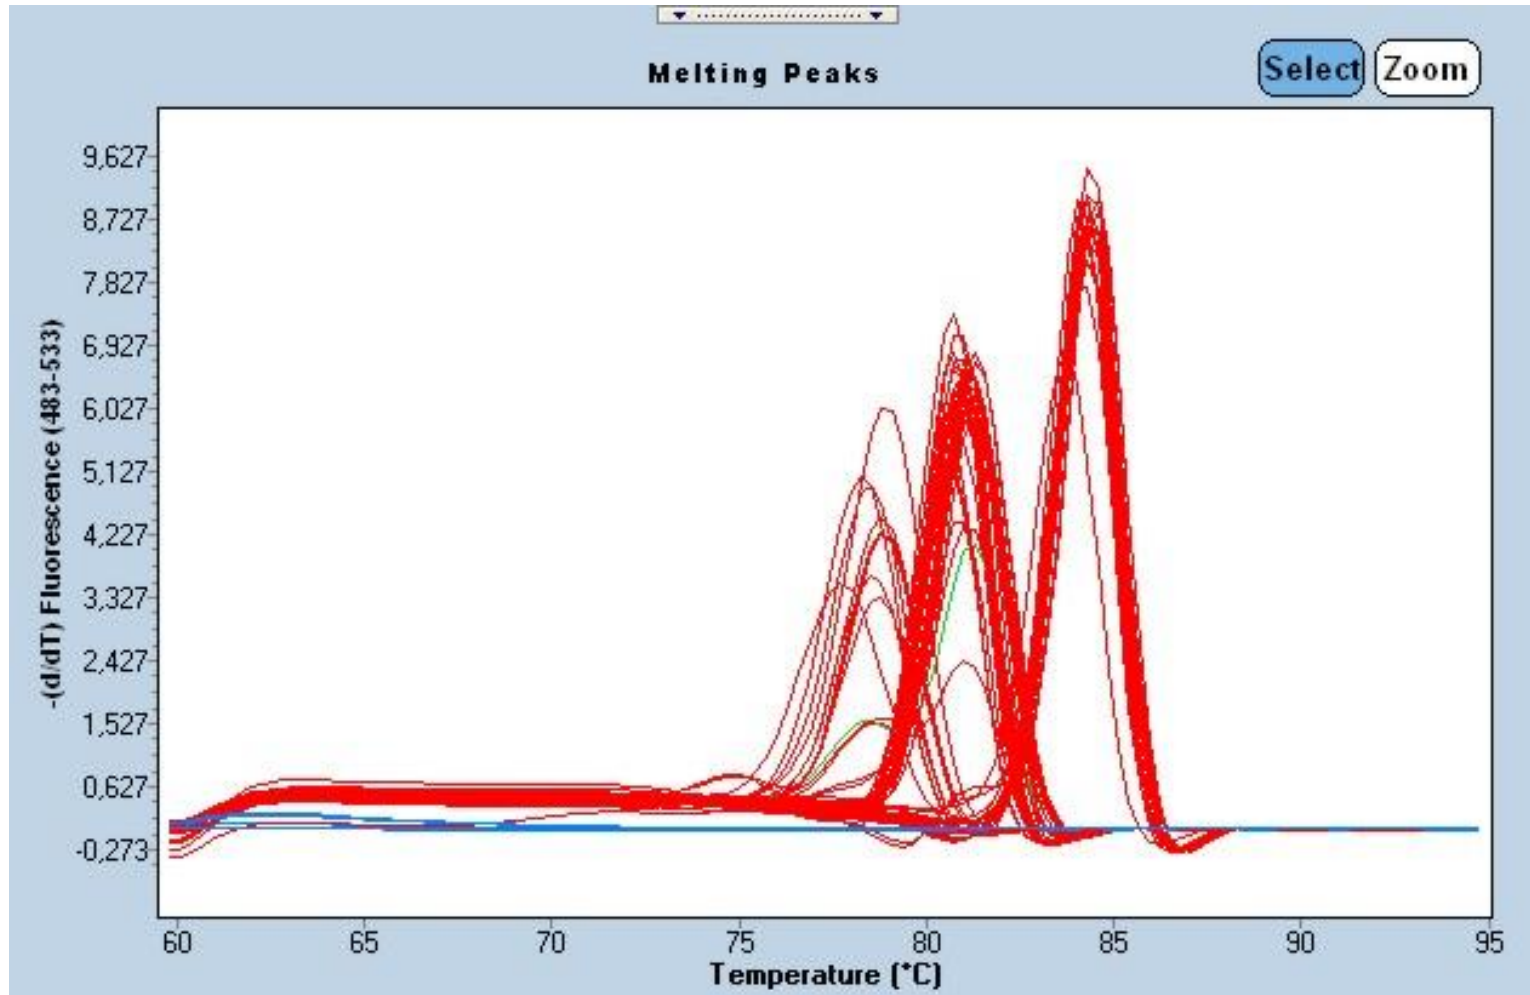



Analysis of melting curves

Pure, specific qPCR product

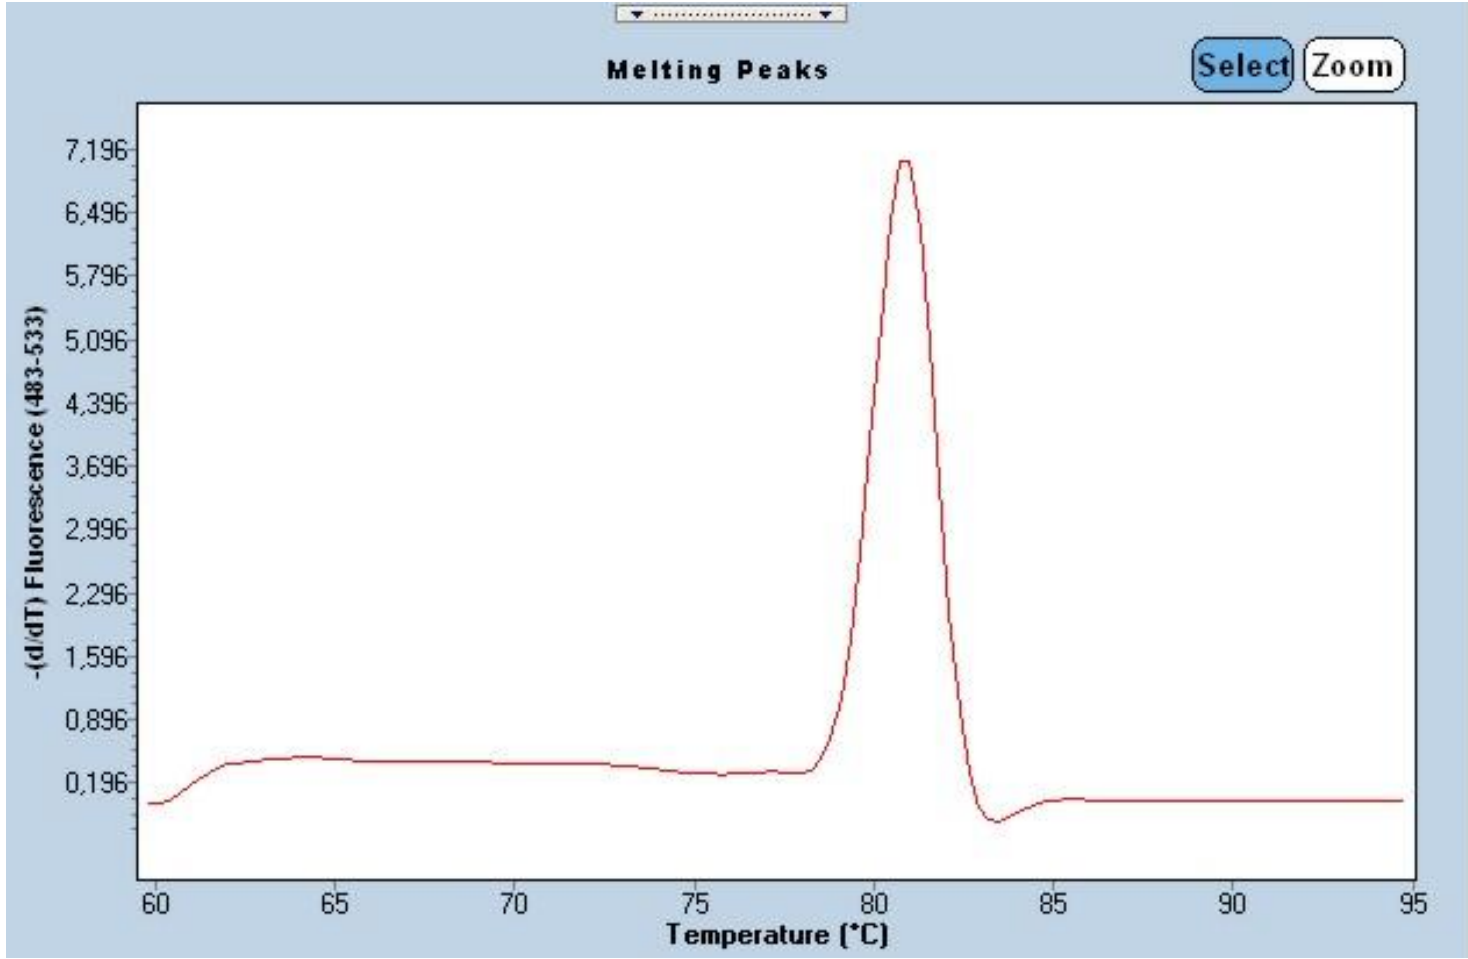



Analysis of melting curves

Non-specific products

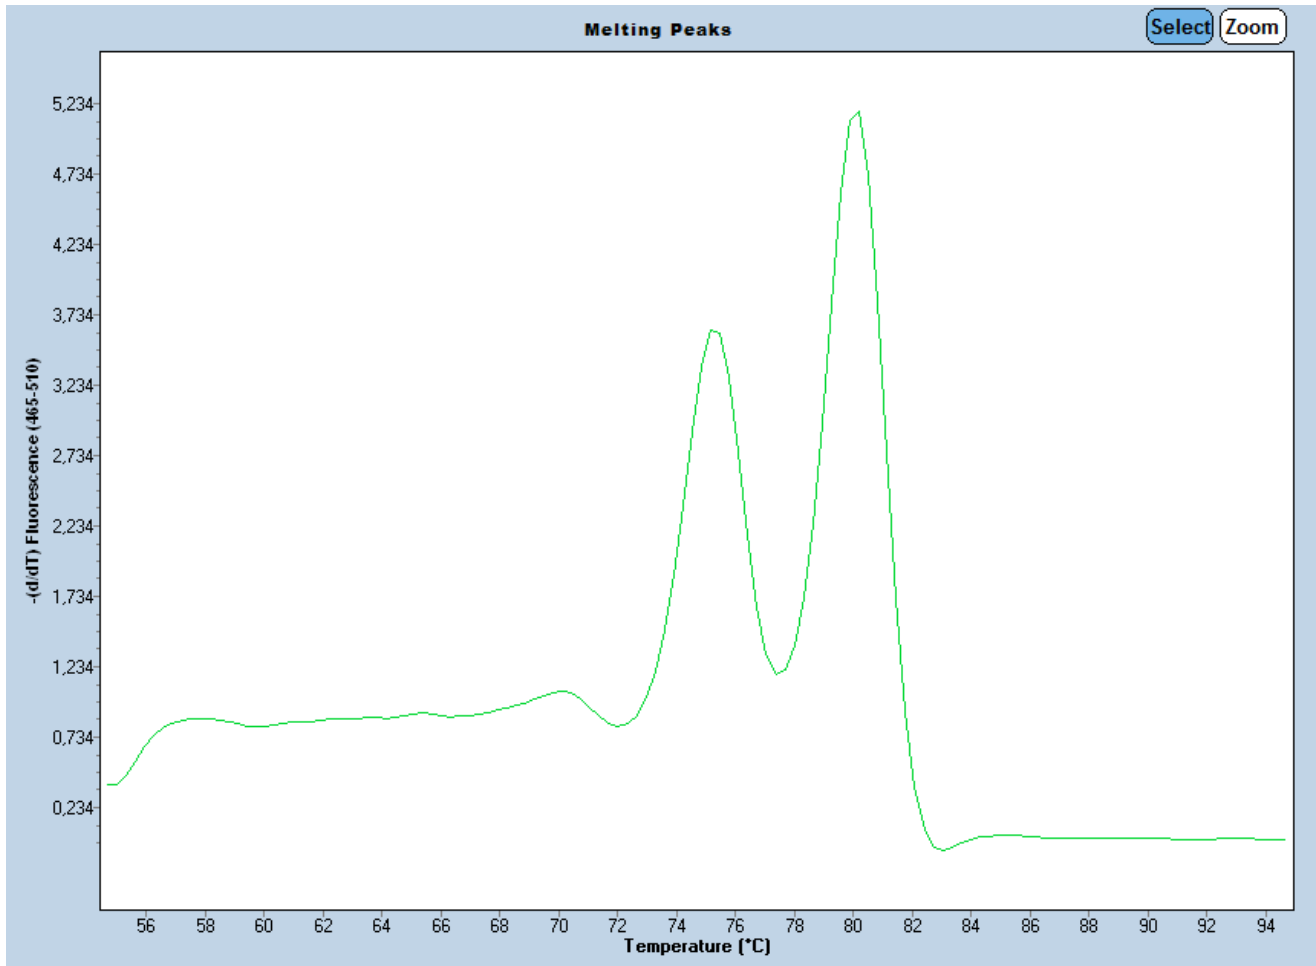

Analysis of melting curves

The primer-dimer problem

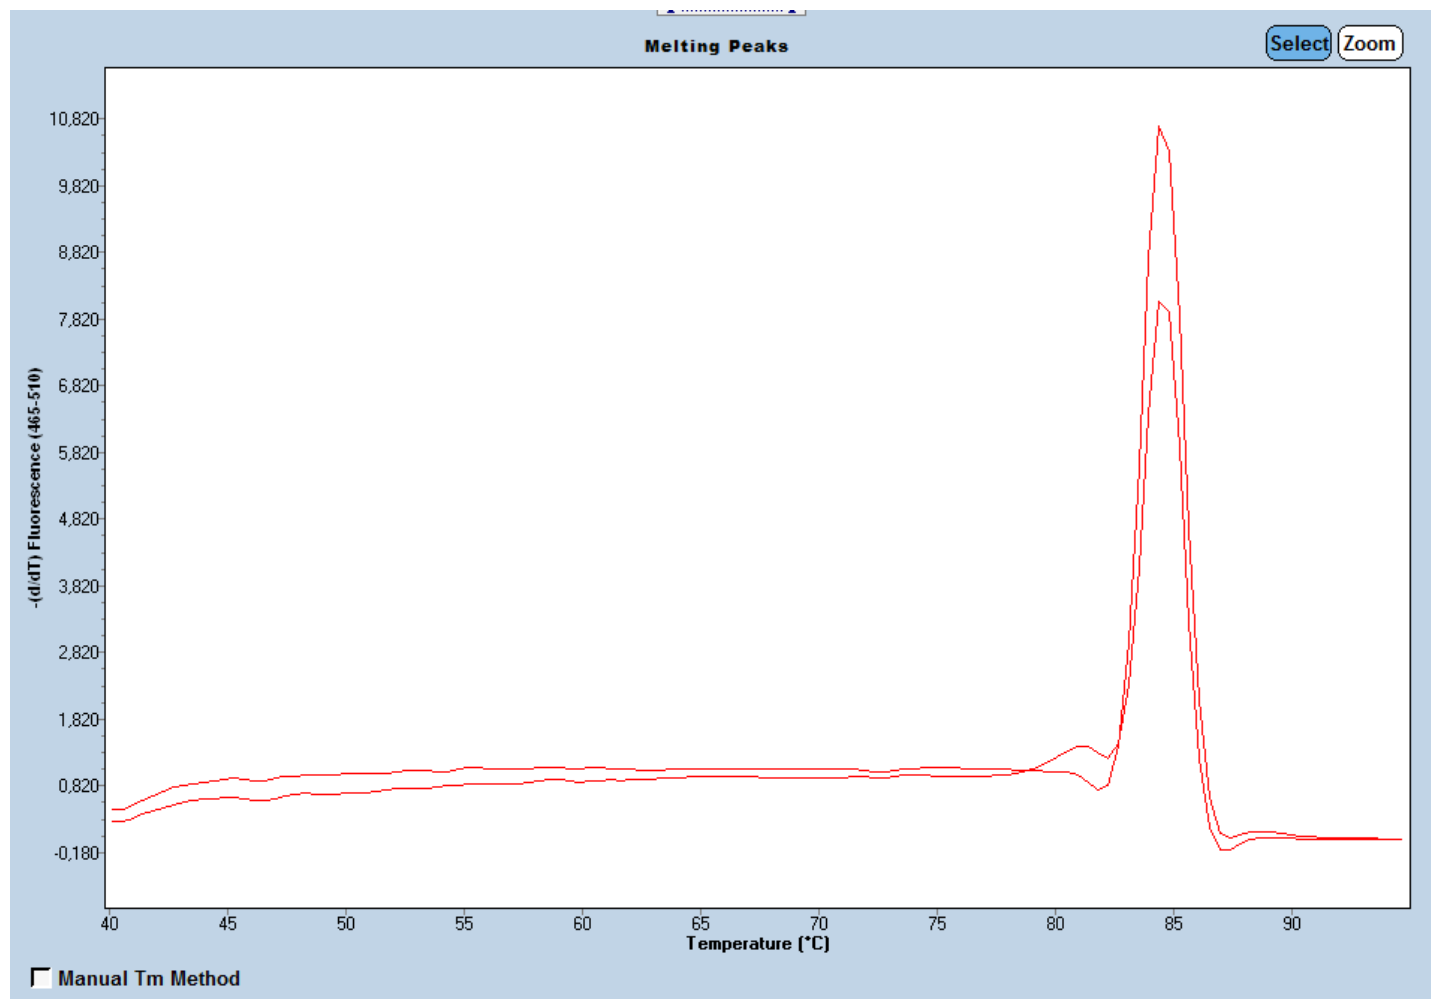


Analysis of melting curves


Do not blindly believe the melting curves!!!

A longer AT-rich product can have the same T_m as a shorter GC-rich one!!!

Always check the products for each new primer pair on a high-resolution gel! At least once, at the "reaction setup" stage.



Standardization




Reference gene selection

THERE IS NO "PERFECT" REFERENCE GENE!!!

- Equal number of RNA copies in all cells
- Expressed in all cells
- Expressed at a medium level

- At least 2 different reference genes should be used!
Better 3 to even 5!!!
- Standardize against the geometric mean for the reference.
- Genes should be selected **EXPERIMENTALLY** from a larger group!!!

Vandesompele et al, Genome Biology, 2002,



Statistical analysis of Cq value variation for reference genes




*Vandesompele et al.,
Genome Biology, 2002,*

Nowadays geNorm is part of Biogazelle's qbase+ software for quantitative PCR data-analysis

<https://www.qbaseplus.com/>

| Change Data | GAPD | ACTB | HPRT1 | UBC | YHWAZ | Normalisation |
|-------------------|--------------|--------------|--------------|--------------|--------------|---------------|
| FIB1 | 0,516257 | 0,499303 | 0,482906 | 0,447207 | 0,572560 | 0,5828 |
| FIB2 | 0,287796 | 0,238713 | 0,313899 | 0,221805 | 0,351638 | 0,2787 |
| FIB3 | 0,160974 | 0,262108 | 0,147588 | 0,177935 | 0,306647 | 0,2824 |
| FIB4 | 0,462392 | 0,151078 | 0,284928 | 0,372176 | 0,221805 | 0,2774 |
| FIB5 | 0,694914 | 0,678860 | 0,765572 | 0,572560 | 0,851906 | 0,7866 |
| FIB6 | 0,001146 | 0,000160 | 0,000765 | 0,000377 | 0,000690 | 0,0005 |
| FIB7 | 0,487767 | 0,574475 | 0,512821 | 0,418316 | 0,685694 | 0,5285 |
| FIB8 | 0,192781 | 0,183976 | 0,151584 | 0,181536 | 0,169808 | 0,1753 |
| FIB9 | 0,393914 | 0,281148 | 0,386101 | 0,411390 | 0,342369 | 0,3597 |
| FIB10 | 0,011902 | 0,005503 | 0,009390 | 0,010310 | 0,012347 | 0,0895 |
| FIB11 | 0,016844 | 0,008107 | 0,013740 | 0,022522 | 0,023837 | 0,0159 |
| FIB12 | 0,011059 | 0,014301 | 0,011902 | 0,017709 | 0,015443 | 0,0139 |
| FIB13 | 0,008438 | 0,007141 | 0,009676 | 0,010589 | 0,014206 | 0,0097 |
| FIB14 | 0,593982 | 0,697238 | 0,624490 | 0,550071 | 0,708977 | 0,6328 |
| FIB15 | 0,283978 | 0,196683 | 0,218133 | 0,445716 | 0,234760 | 0,2637 |
| FIB16 | 0,572560 | 0,423941 | 0,544589 | 0,414147 | 0,528466 | 0,4923 |
| FIB17 | 0,720913 | 0,990033 | 0,877896 | 0,880833 | 0,983443 | 0,8858 |
| FIB18 | 0,514536 | 0,504330 | 0,533786 | 0,590028 | 0,467047 | 0,5284 |
| FIB19 | 1,00E+00 | 1,00E+00 | 1,00E+00 | 1,00E+00 | 1,00E+00 | 1,0008 |
| FIB20 | 0,399211 | 0,316002 | 0,283978 | 0,441273 | 0,349298 | 0,3535 |
| M < 1.5 | 0.513 | 0.664 | 0.432 | 0.523 | 0.475 | |


<https://genorm.cmgg.be/>




Reference gene selection

Alternatively...

- Trust published data, e.g., for human cells: GAPDH, albumin, actin, tubulin, cyclophilin, microglobulin, 18S or 28S rRNA... though risky
- e.g. <https://www.gene-quantification.de/hkg.html#refgenes>
- Or use commercial primer panels (only possible for some model organisms)




Layout design of the experiment



RT error accumulation


$$SD_{mRNA}^2 = SD_{RT}^2 + SD_{QPCR}^2$$




2 experimental designs

- The **"sample maximization"** method: as many different samples as possible analyzed in a single run of the instrument. That is, different genes analyzed in different reactions (preferred in routine research work - many culture conditions, many mutants, etc.).
- The **"gene maximization"** method: as many different primer pairs as possible during a single run of the device (preferred in commercial diagnostic kits: one patient - one reaction plate for multiple genes)
- **Whichever method you choose, use IRC**

Hellemans et al, Genome Biology, 2007,




How many biological repeats, RT, qPCR?

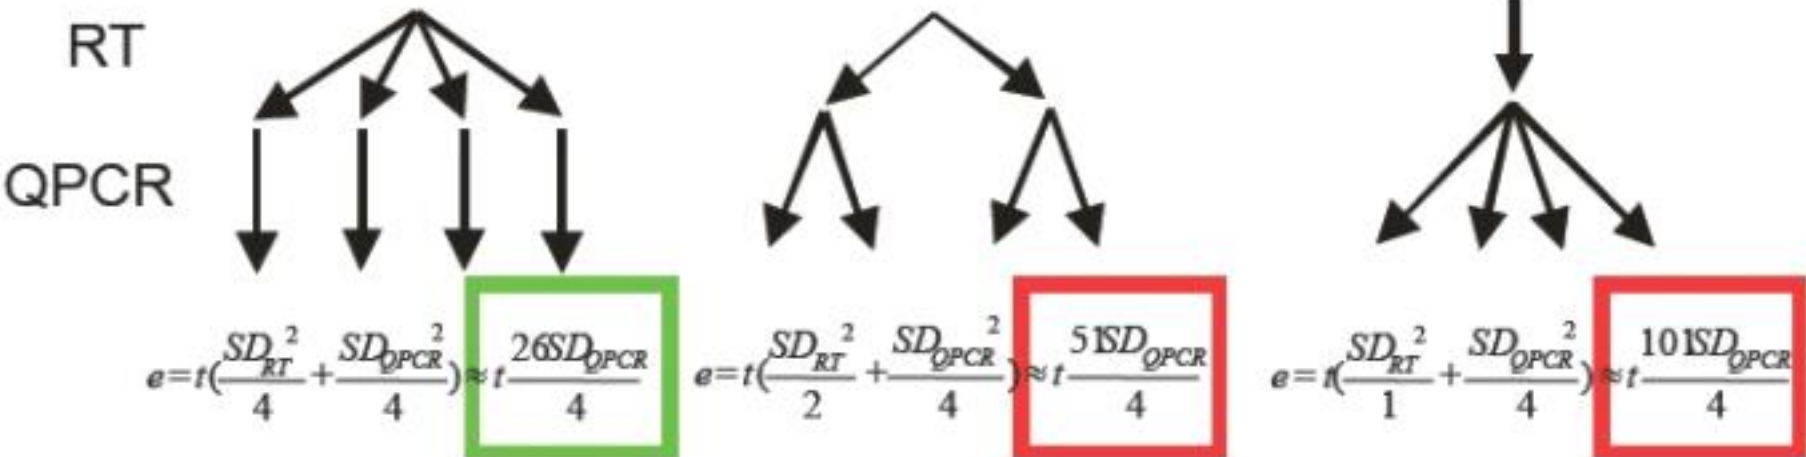


Ref: Ståhlberg *et al.* Properties of the reverse transcription reaction in mRNA quantification Clin Chem 2004;50:3

TATAA Biocenter




Optimization of qPCR reactions




Optimization of qPCR reactions


- **Optimization of reaction conditions: concentrations of dNTPs, Mg²⁺, primers, SYBR Green - currently difficult because most "mixes" are "ready to use" and 2X concentrated.**
- **Program optimization: temperature and time of primers annealing and synthesis.**
- **4-step PCR (SYBR Green fluorescence measurement above T_m for product) or 2-step PCR (95 and 72°C only – common temperature of primer annealing and DNA synthesis)**
- **"touch-down" PCR, "hot-start" DNA polymerase**
- **The fastest way to optimize is to redesigning oligonucleotides**




PRIMERS T_m: PREDICTED vs DETERMINED EXPERIMENTALLY

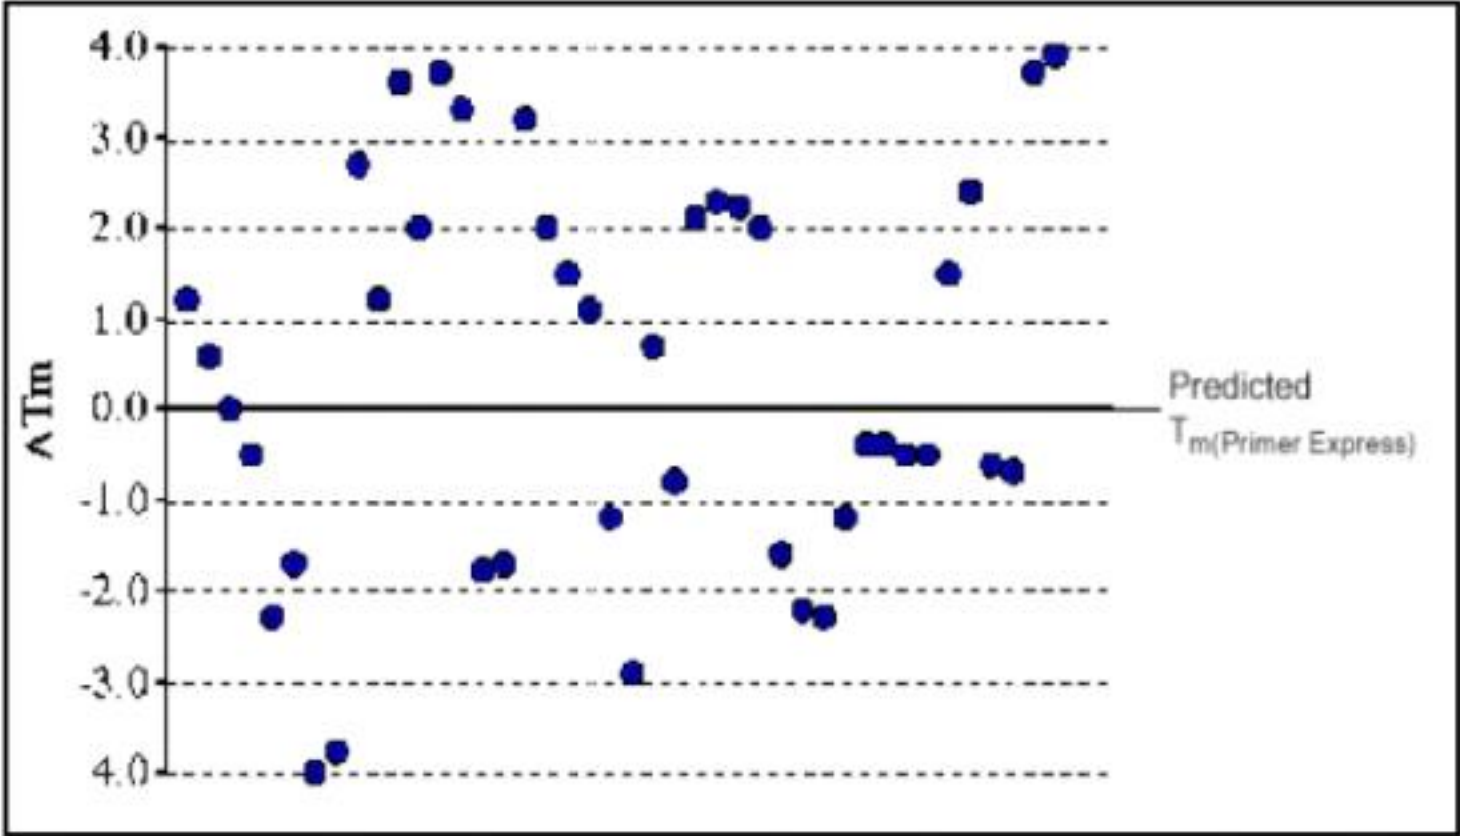

Source: ABI User Bulletin 6 ABI PRISM® Sequence Detection System



Take home message!



Always keep standards!!!

Clinical Chemistry 55:4
611–622 (2009)

Special Report

The MIQE Guidelines: Minimum Information for Publication of Quantitative Real-Time PCR Experiments

Stephen A. Bustin,^{1*} Vladimir Benes,² Jeremy A. Garson,^{3,4} Jan Hellemans,⁵ Jim Huggett,⁶
Mikael Kubista,^{7,8} Reinhold Mueller,⁹ Tania Nolan,¹⁰ Michael W. Pfaffl,¹¹ Gregory L. Shipley,¹²
Jo Vandesompele,⁵ and Carl T. Wittwer^{13,14}

<http://www.gene-quantification.de/miqe.html>

Methods 50 (2010) S1–S5



Contents lists available at ScienceDirect

Methods

journal homepage: www.elsevier.com/locate/ymeth




Mini-review

A practical approach to RT-qPCR—Publishing data that conform to the MIQE guidelines ☆☆☆

Sean Taylor, Michael Wakem, Greg Dijkman, Marwan Alsarraj, Marie Nguyen *

Bio-Rad Laboratories, Inc., Hercules, CA 94547, USA





www.Gene-Quantification.info 21st Anniversary!
The Reference in qPCR & dPCR - Academic & Industrial Information Platform

Founded February 2002 – Since 21 years, the Gene Quantification platform describes and summarises all technical aspects involved in quantitative gene expression analysis using **real-timePCR (qPCR) & digital-PCR (dPCR) & Next Generation Sequencing**. It presents the majority of [new and innovative qPCR & dPCR applications](#), chemistries, methods, data analysis algorithms, [MIQE & QC strategies](#), cyclers, kits, dyes, analysis methods, interesting events & workshops, and services involved. Please browse our [page directory](#) with all essential keywords or the [qPCR platform](#), a summary of commercial and academic institutions presenting their PCR related tools.

Amplify your knowledge in qPCR, dPCR and NGS! Follow our streaming server presenting 500 talks => [eConferences.de](#)



[MIQE iBook ... 5th eds](#)
[Books eBooks ePub](#)
[eConferences & Webinars](#)
[Quantification Strategy](#)
[Normalisation](#)
[qPCR & Optimisation](#)
[Bioinformatics & Statistics](#)
[Software Downloads](#)
[RNAi – RNA interference](#)
[Gene Quantification Events](#)
[digital-PCR & qPCR Array](#)
[Cyclers & Robotics](#)
[RNA & RT & RNA QC](#)
[Dyes & HRM dyes](#)
[Liquid Biopsy & Biomarkers](#)
[Molecular Physiology](#)
[qPCR Efficiency](#)
[qPCR & dPCR applications](#)
[GQ info portal](#)


[EV & Exosomes & EV RNA / Liquid Biopsy / Biomarker Discovery / Transcriptional Biomarkers](#)
[qPCR Platform / Protocols / Methods / Translation / ASIA portal / GQ Page Directory](#)
"free access" to 500 recorded talks [Gene Quantification Events 2010-2023](#) / [Talks / Webinars](#)
Quantification strategies: [absolute Quantification & relative Quantification](#) / [qPCR Evolution](#)
[RT-qPCR normalisation strategies & microRNA / Genom / BestKeeper / RefGenes](#)
[real-time PCR / interesting reviews / MIQE & Apps & iBook / Primer-Resources & Algorithms](#)
[Big Data in Biology / data analysis / Regulatory Networks / data clustering / Integrated Analysis](#)
[REST \(main page\) / REST-2009 / RDML / RefGenes / GenEx 7.0 ... FREE DOWNLOAD](#)
[siRNA / saRNA / microRNA & microRNA normalisation / mirtron / qPCR statistics](#)
[impressions GQ2023 / qPCR dPCR NGS 2023 / MicroGenomics 2023 / eConferences / previous Events](#)
[digital-PCR ... UPDATE / MIQE & dPCR / qPCR array / normalisation and analysis software](#)
real-time PCR hardware: [overview of qPCR cyclers](#) / [qPCR robotics](#) / [page statistics](#)
[reverse transcription / mRNA transcript analysis ... UPDATE / RNA QC & RNA / DNA integrity](#)
detection dyes, probes, and chemistries in real-time PCR / [HRM dyes / Chips & Lab-on-Chip](#)
[Exosomes / EV & exRNA ... UPDATE / CNA / microRNA / Transcriptional Biomarkers](#)
[CNA / HRM / CNV / microRNA / siRNA / saRNA / RNAi / digital-PCR / single-cell qPCR](#)
determination of [real-time qPCR efficiency](#) by various methods [new efficiency papers!](#)
[EVs & Exosomes / circulating nucleic acids / digital-PCR / single-cell handling / single-cell qPCR](#)
[microRNA / CNV / microRNA transfer / HRM / RNAi / siRNA / saRNA / Liquid Biopsy](#)



qPCR NEWS The reference in qPCR


powered by [www.Gene-Quantification.info](#)

Gene Quantification Newsletter is sponsored by **GenEx**




SUMMARY


- **qPCR is a highly efficient, rapid and accurate method for nucleic acid quantification**
- **Enables low and medium throughput gene expression studies**
- **qPCR is based on real-time detection of DNA using fluorescent dyes**
- **$(1+E)^n = 2^n$ if $E=100\%$ ($2^{\Delta\Delta Ct}$)**
- **Quality control and correct design of the experiment are crucial!!!**








Thank you for your attention!



Supplement 1- examples of qPCR application



Actin mRNA precursor qPCR *By David Barras*

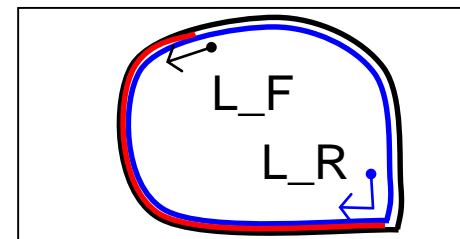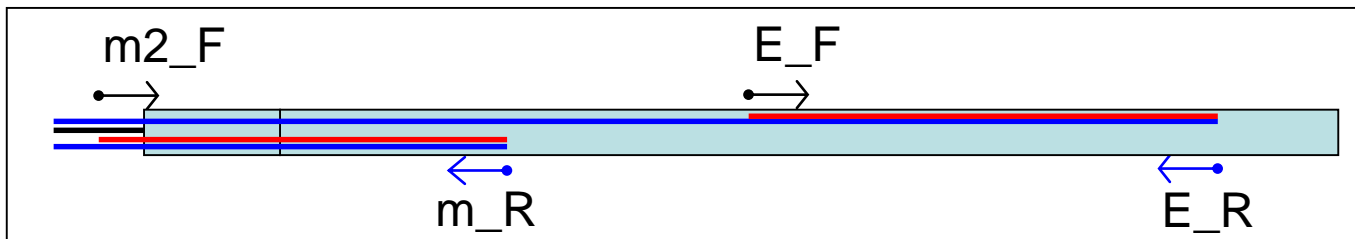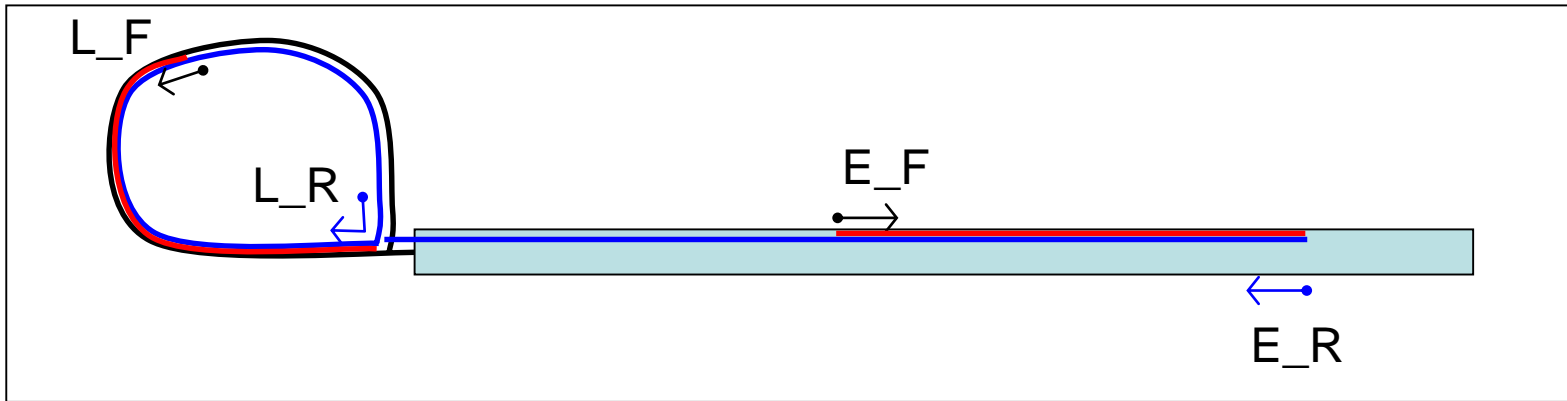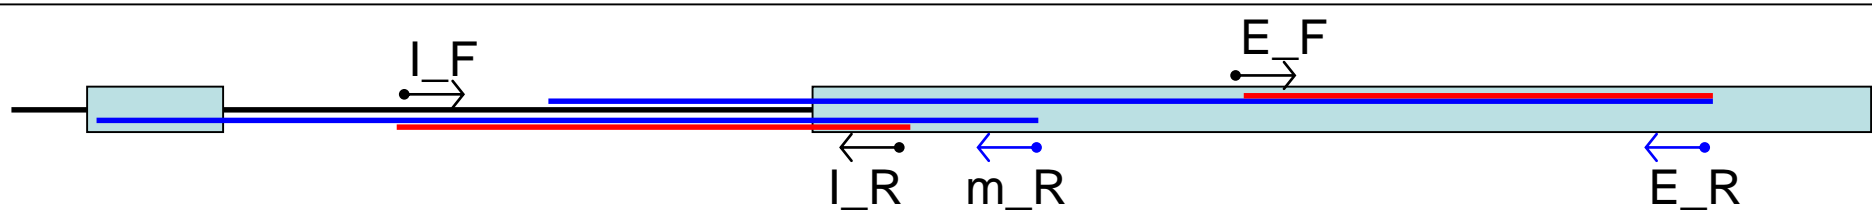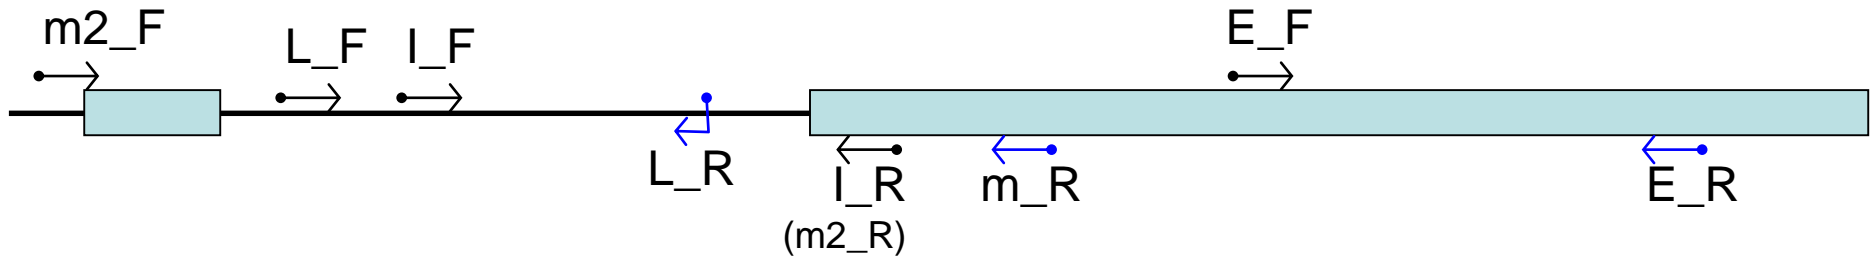

Single cel qPCR




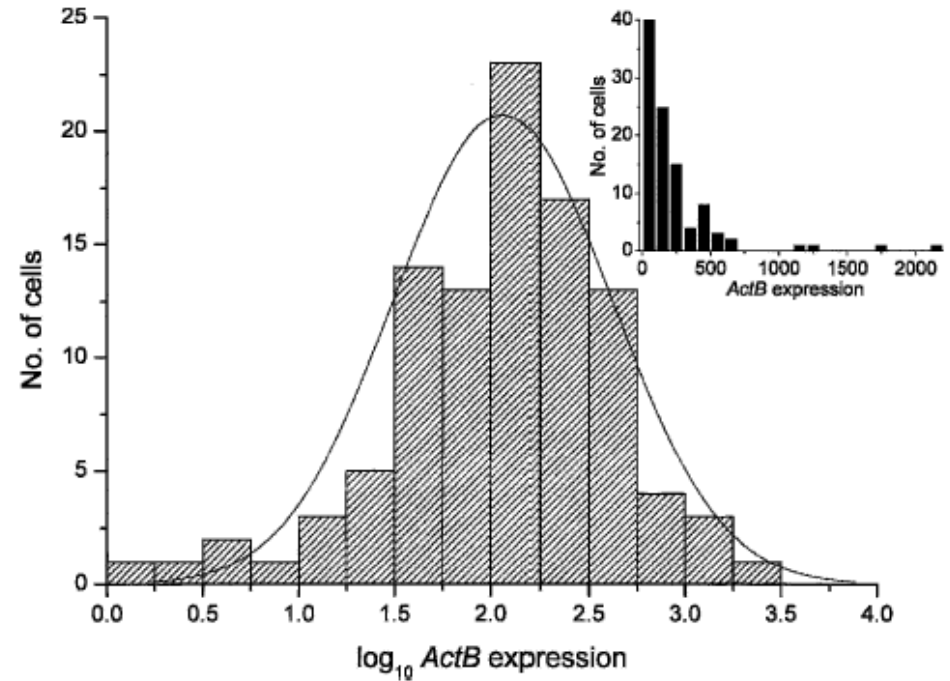


Figure 1. Histograms showing the expression levels of 96 cells expressing *ActB* in logarithmic and linear scale (*inset*). Logarithms of transcript levels are mean-centered for the two glucose concentrations. Solid line describes lognormal distribution centered on the geometric mean (2.06) of the *ActB* expression levels. *Inset* shows histogram of the expression levels in linear scale.


Bengtsson M, Stahlberg A, Rorsman P, Kubista M. *Genome Res.* 2005 Oct;15(10):1388-92.

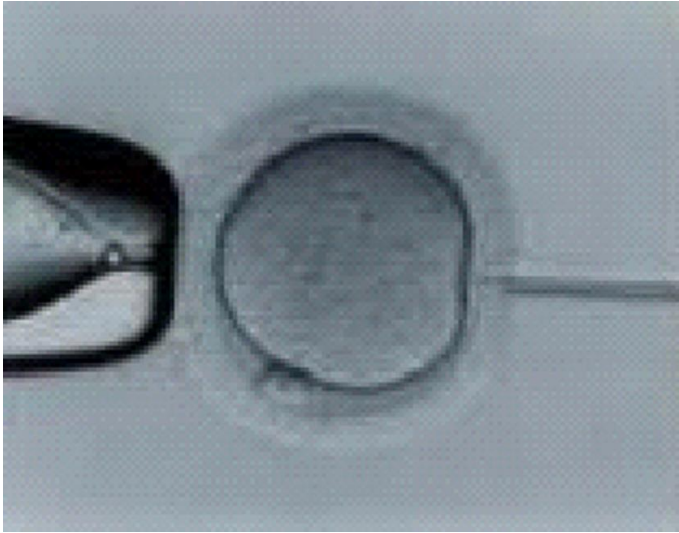

Digital PCR - dPCR

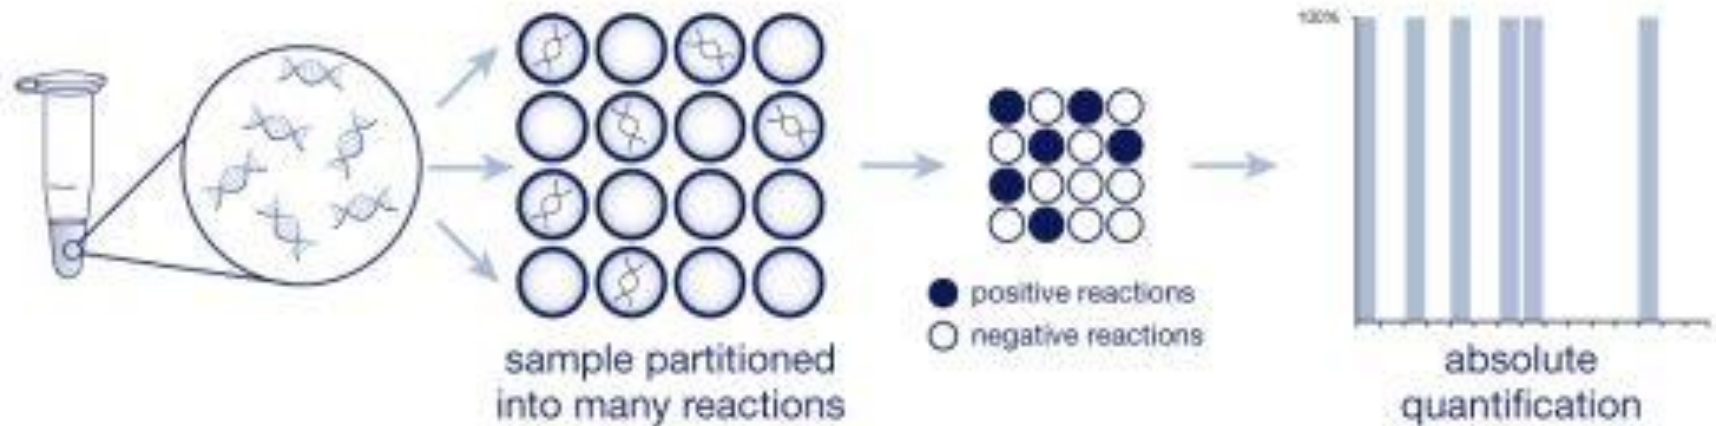

| | Absolute Quantification (Digital PCR Method) | Absolute Quantification (Standard Curve Method) |
|-----------------|---|--|
| Overview | In absolute quantification using Digital PCR, no known standards are needed. The target of interest can be directly quantified with precision determined by number of digital PCR replicates. Quantify copies of rare allele present in heterogenous mixtures. | In absolute quantification using the Standard Curve Method, you quantitate unknowns based on a known quantity. First you create a standard curve; then you compare unknowns to the standard curve and extrapolate a value. |
| Example | Count the number of cell equivalents in sample by targeting genomic DNA. Determine absolute number of viral copies present in a given sample without reference to a standard. | Correlating viral copy number with a disease state. |





dPCR - examples of available platforms

Biorad QX200


- Possible preparation of 1-8 samples simultaneously
- Up to 20,000 reactions / sample
- Up to 96 samples can be read simultaneously

Fluidigm Biomark HD

- (also mass qPCR!)
- From 2,304 to 36,960 independent reactions
- (e.g., 48x48, 192x24, 48x770 layouts)

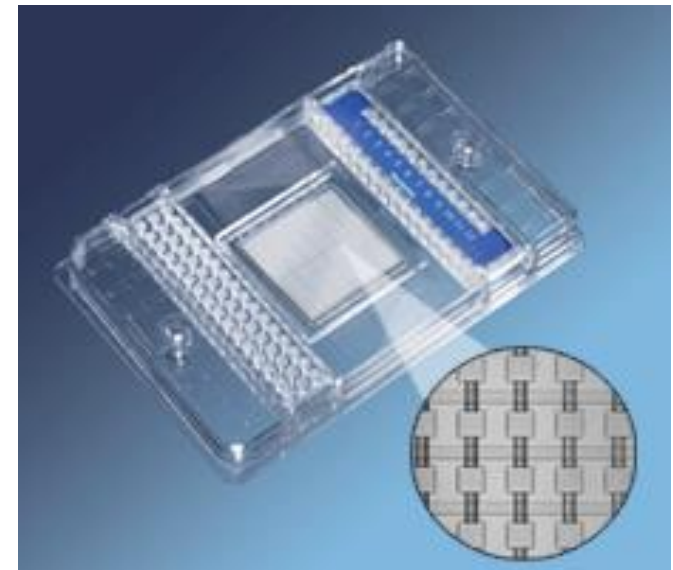


Immuno-qPCR

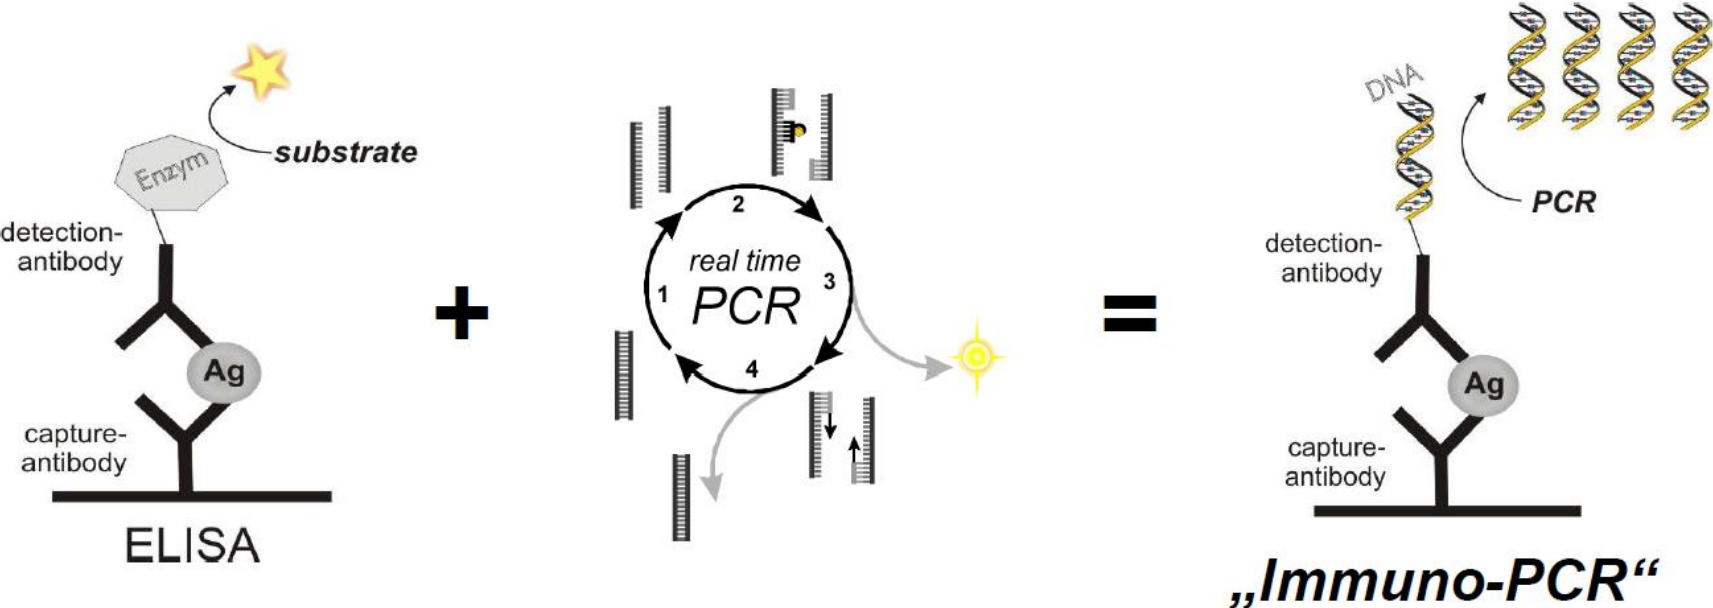


T. Sano, C.L. Smith, C.R. Cantor, *Immuno-PCR: very sensitive antigen detection by means of specific antibody-DNA conjugates*, Science 258 (1992), 120-122


M. Niemeyer; qPCR 2007



Analysis of High-Resolution Melting curves

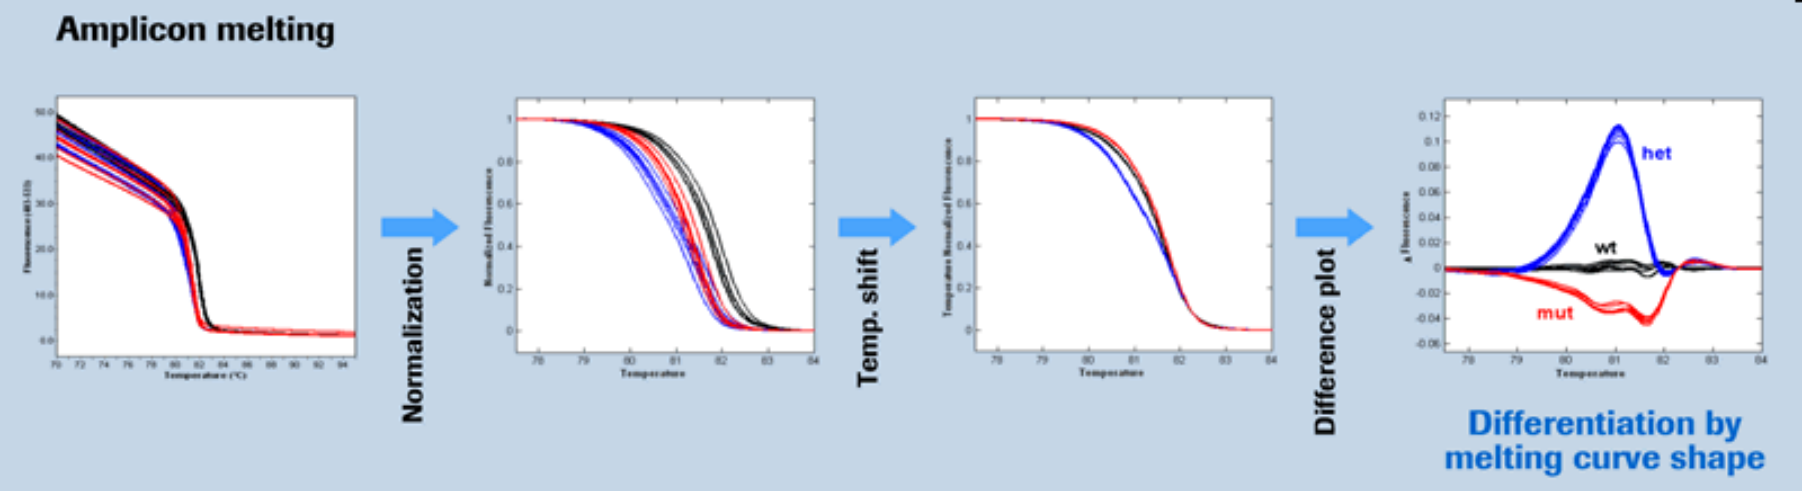


Roche








HRM = High Resolution Melting


- **DNA SATURATING** dyes instead of SYBR Green!!!
- Resolution up to 50 fluorescence measurements / 1°C
- Amplicons of different lengths
- Efficiency doesn't matter: **end-point analysis!**
- Standardization of the template concentration less important




HRM = High Resolution Melting

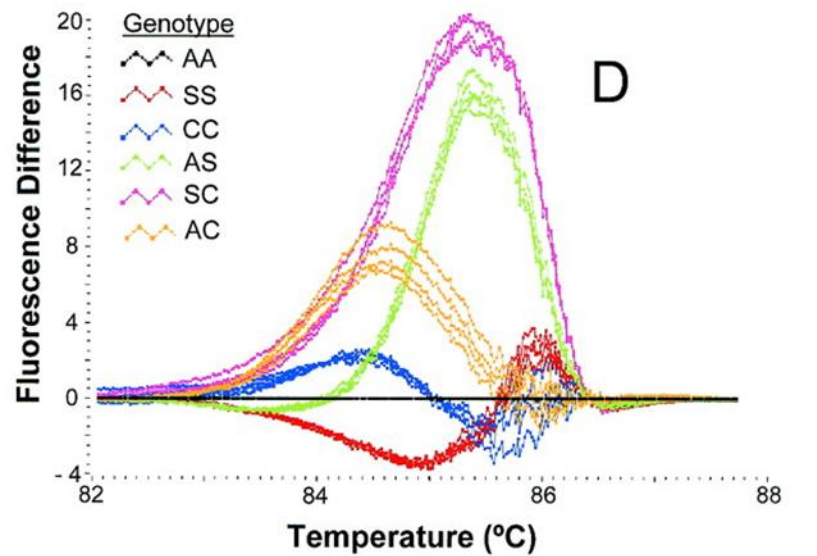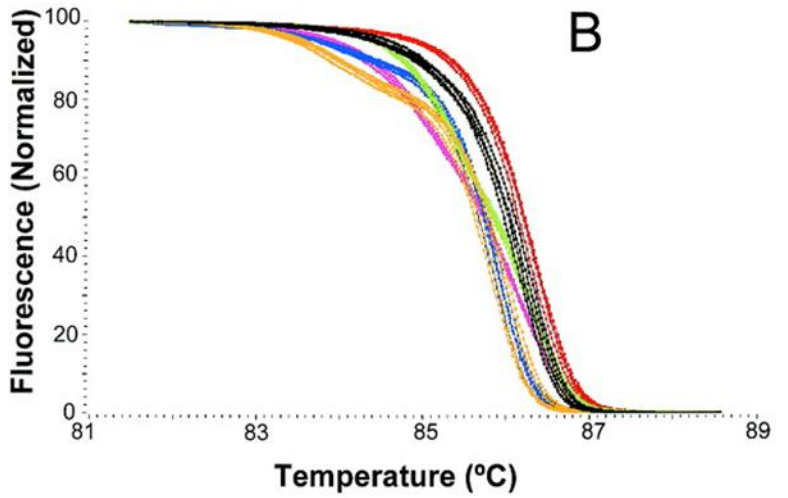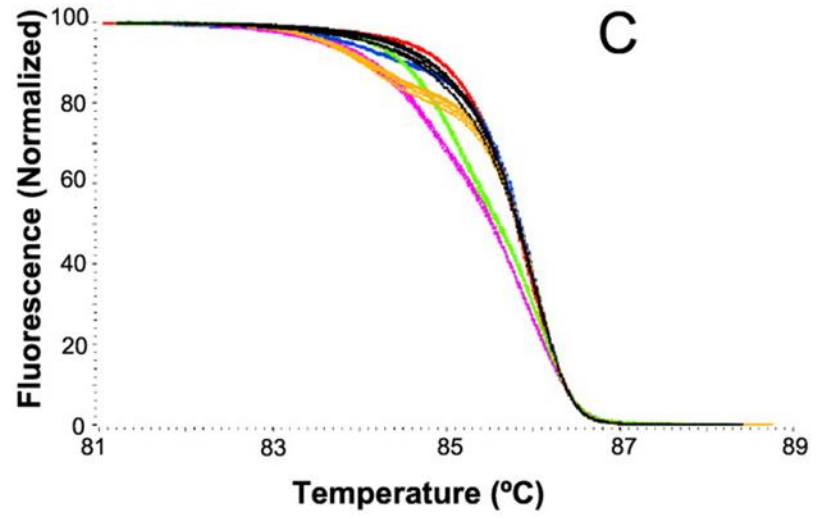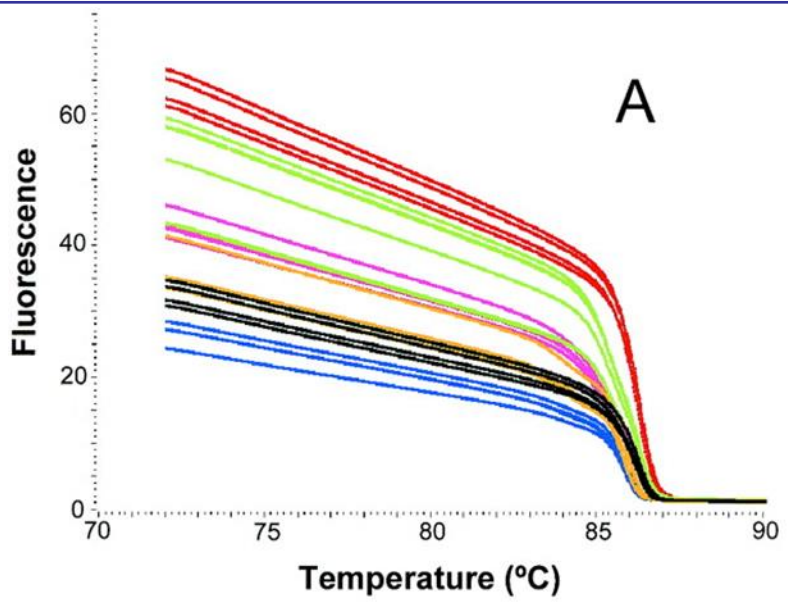


Supplement 2 - using qPCR to analyze chromatin methylation status



DNA methylation silences transcription


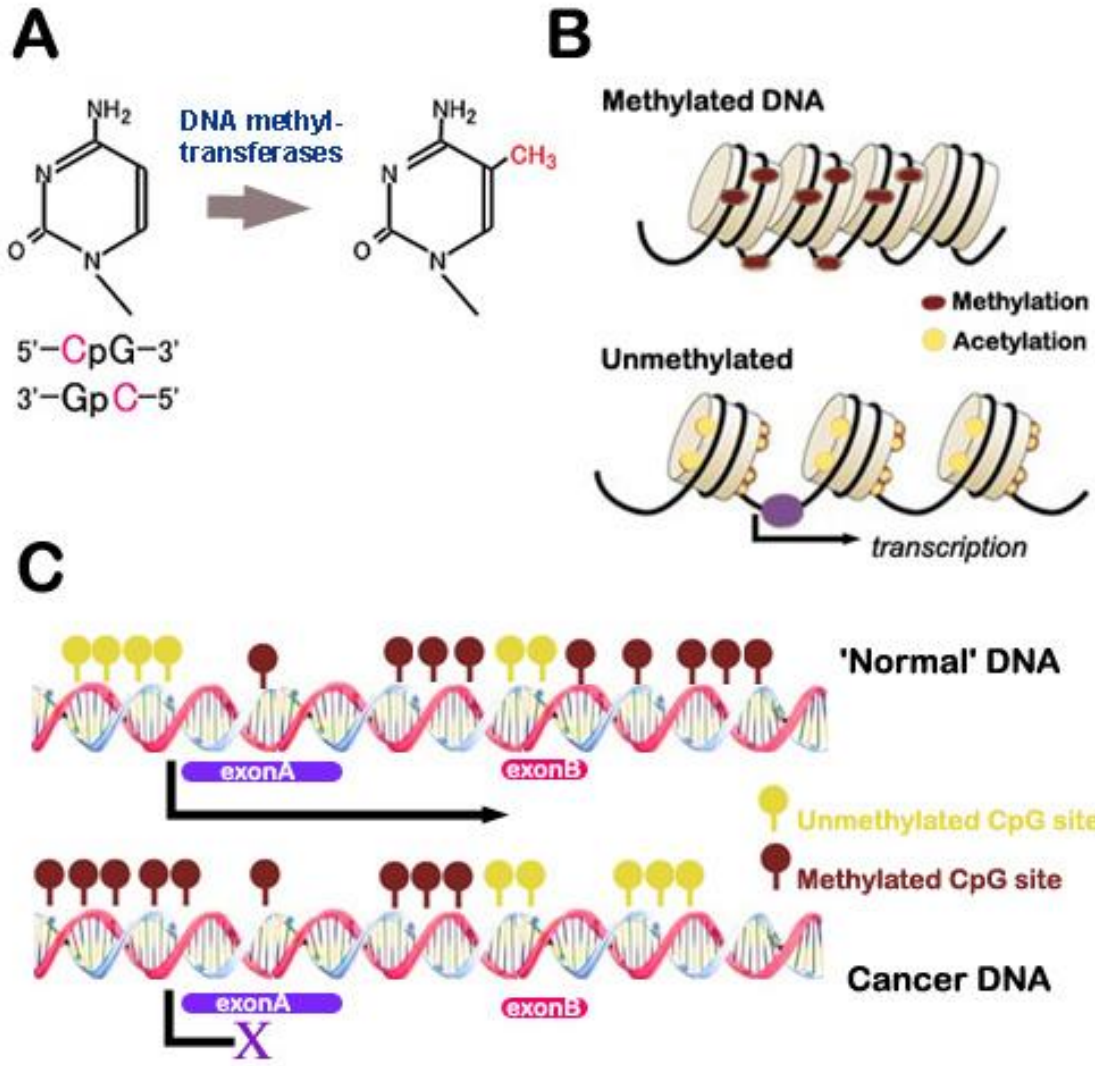


<http://philos.biol.mun.ca>




DNA bisulfite conversions

- Sodium bisulfite converts **CYTOSINE** into **URACYL**
- Does not modify **methyated CYTOSINE**

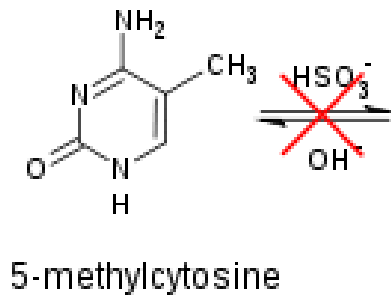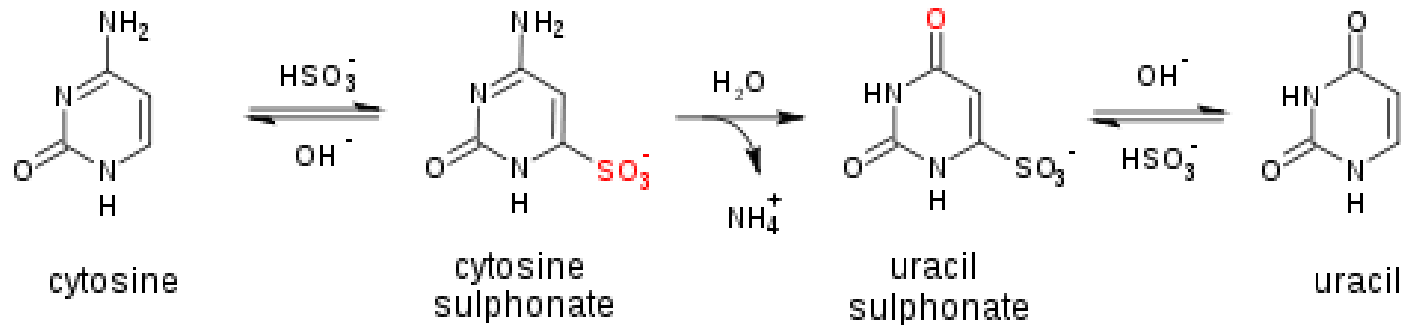


Disadvantages:


- inefficient conversion
- DNA degradation




DNA bisulfite conversions

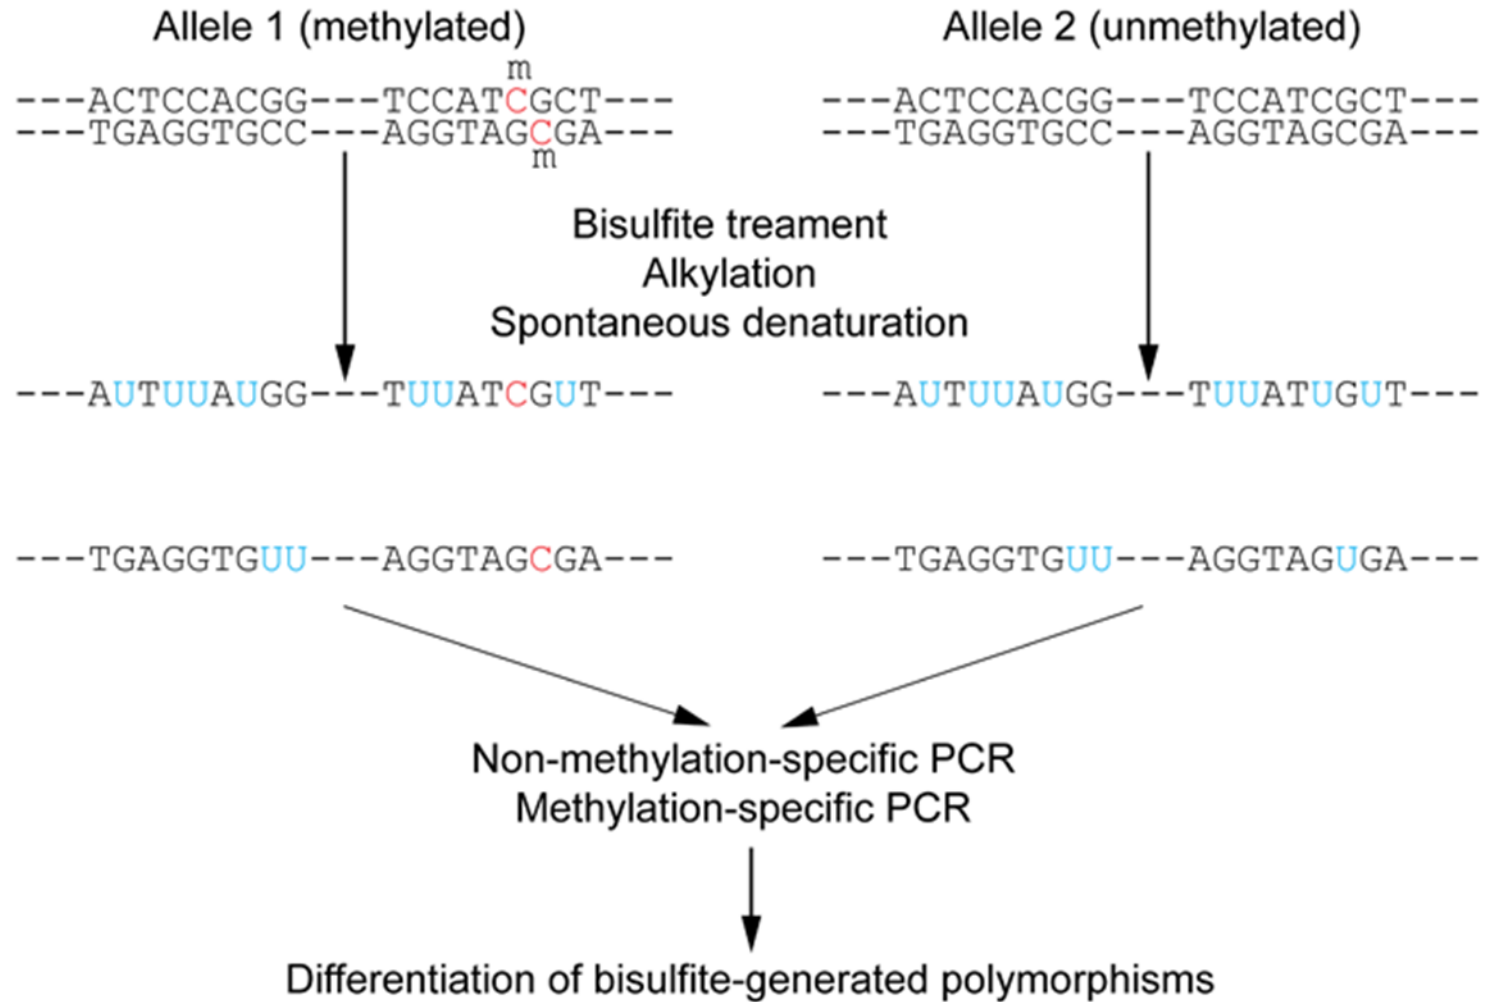


Wikipedia, Bisulfite sequencing





Met-DNA analyses

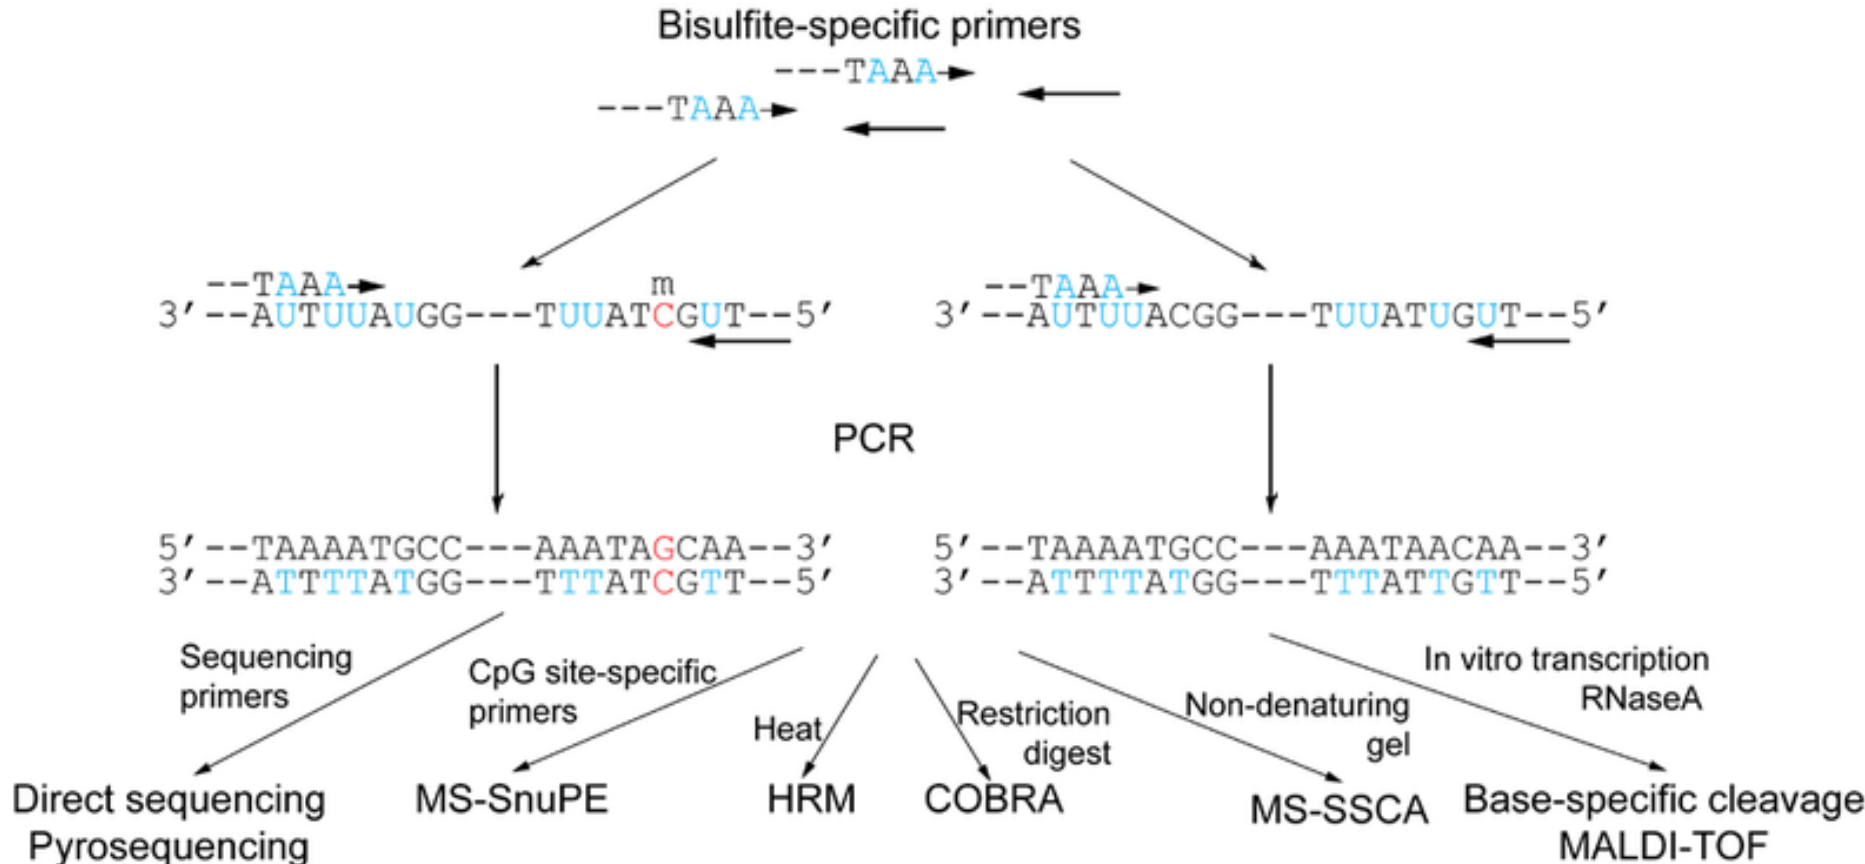


Wikipedia, Bisulfite sequencing



Met-DNA analyses

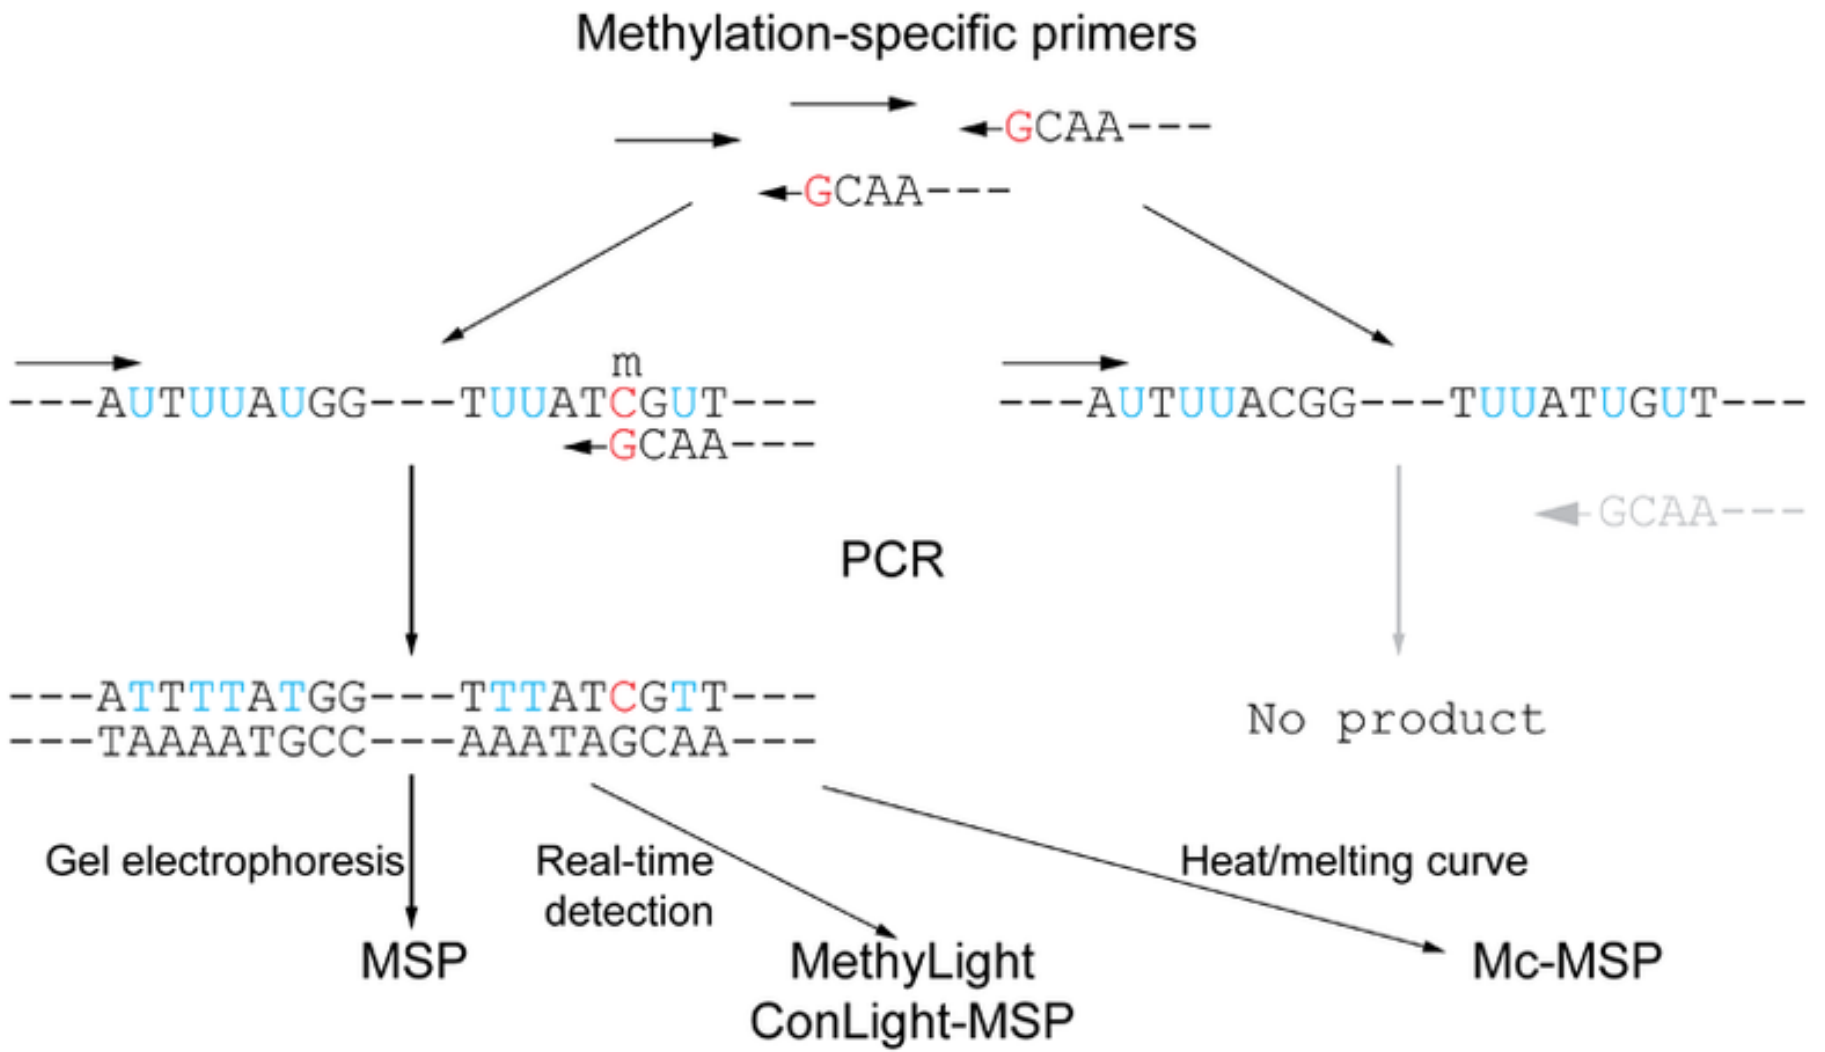

Analysis of methylation status using high-resolution melting curves: MS-HRM

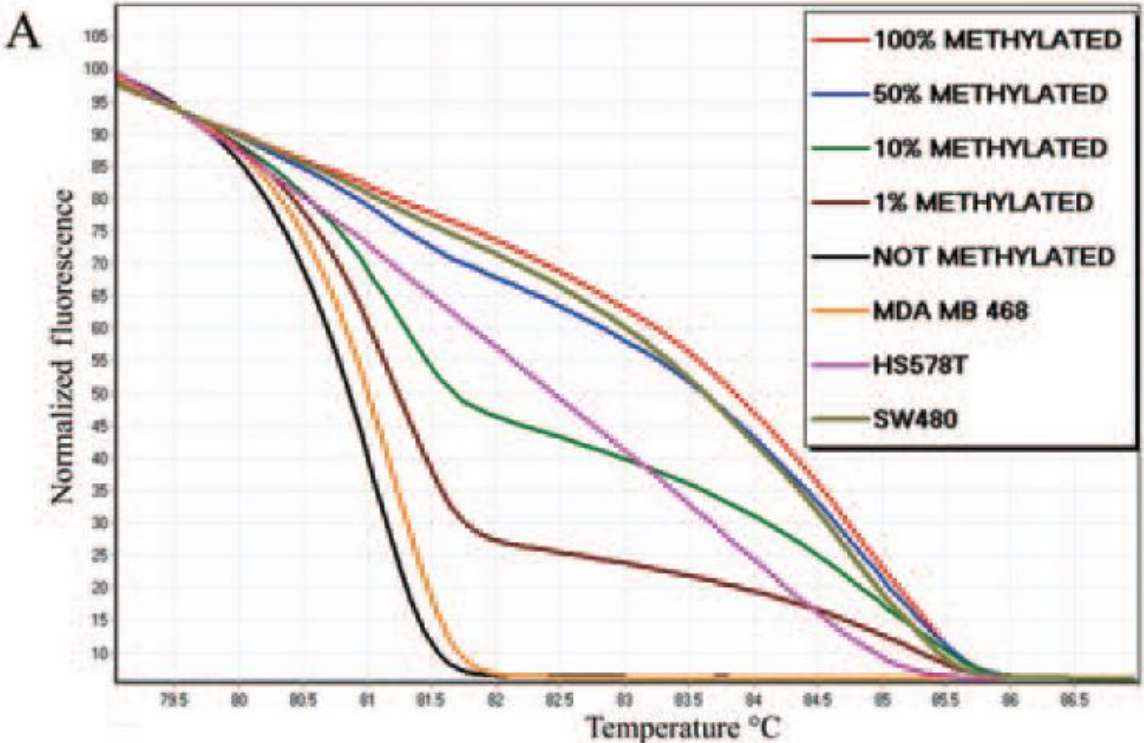

Published online 8 February 2007

Nucleic Acids Research, 2007, Vol. 35, No. 6 e41
doi:10.1093/nar/gkm013

PROTOCOL

Methylation-sensitive high-resolution melting


Tomasz K Wojdacz^{1,2}, Alexander Dobrovic² & Lise Lotte Hansen¹

¹Institute of Human Genetics, University of Aarhus, The Bartholin Building, Wilhelm Meyers Allé, Bygn. 1242, DK-8000 Aarhus C, Denmark. ²Department of Pathology, Peter MacCallum Cancer Centre, Locked Bag 1, A'Becket Street, Victoria 8006, Australia. Correspondence should be addressed to T.K.W. (wojdacz@humgen.au.dk).

Methylation-sensitive high resolution melting (MS-HRM): a new approach for sensitive and high-throughput assessment of methylation

Tomasz K. Wojdacz^{1,2} and Alexander Dobrovic^{1,3,*}

NATURE PROTOCOLS | VOL.3 NO.12 | 2008 | 1903




Supplement 3 - use of RT-qPCR in the diagnosis of coronavirus infections



SARS-CoV-2

<https://www.youtube.com/watch?v=SNvGQJIcQfQ&t=13s>


(in Polish)




Severe acute respiratory syndrome coronavirus 2 (**SARS-CoV-2**) - virus causing **COVID-19** (Coronavirus Disease 2019)

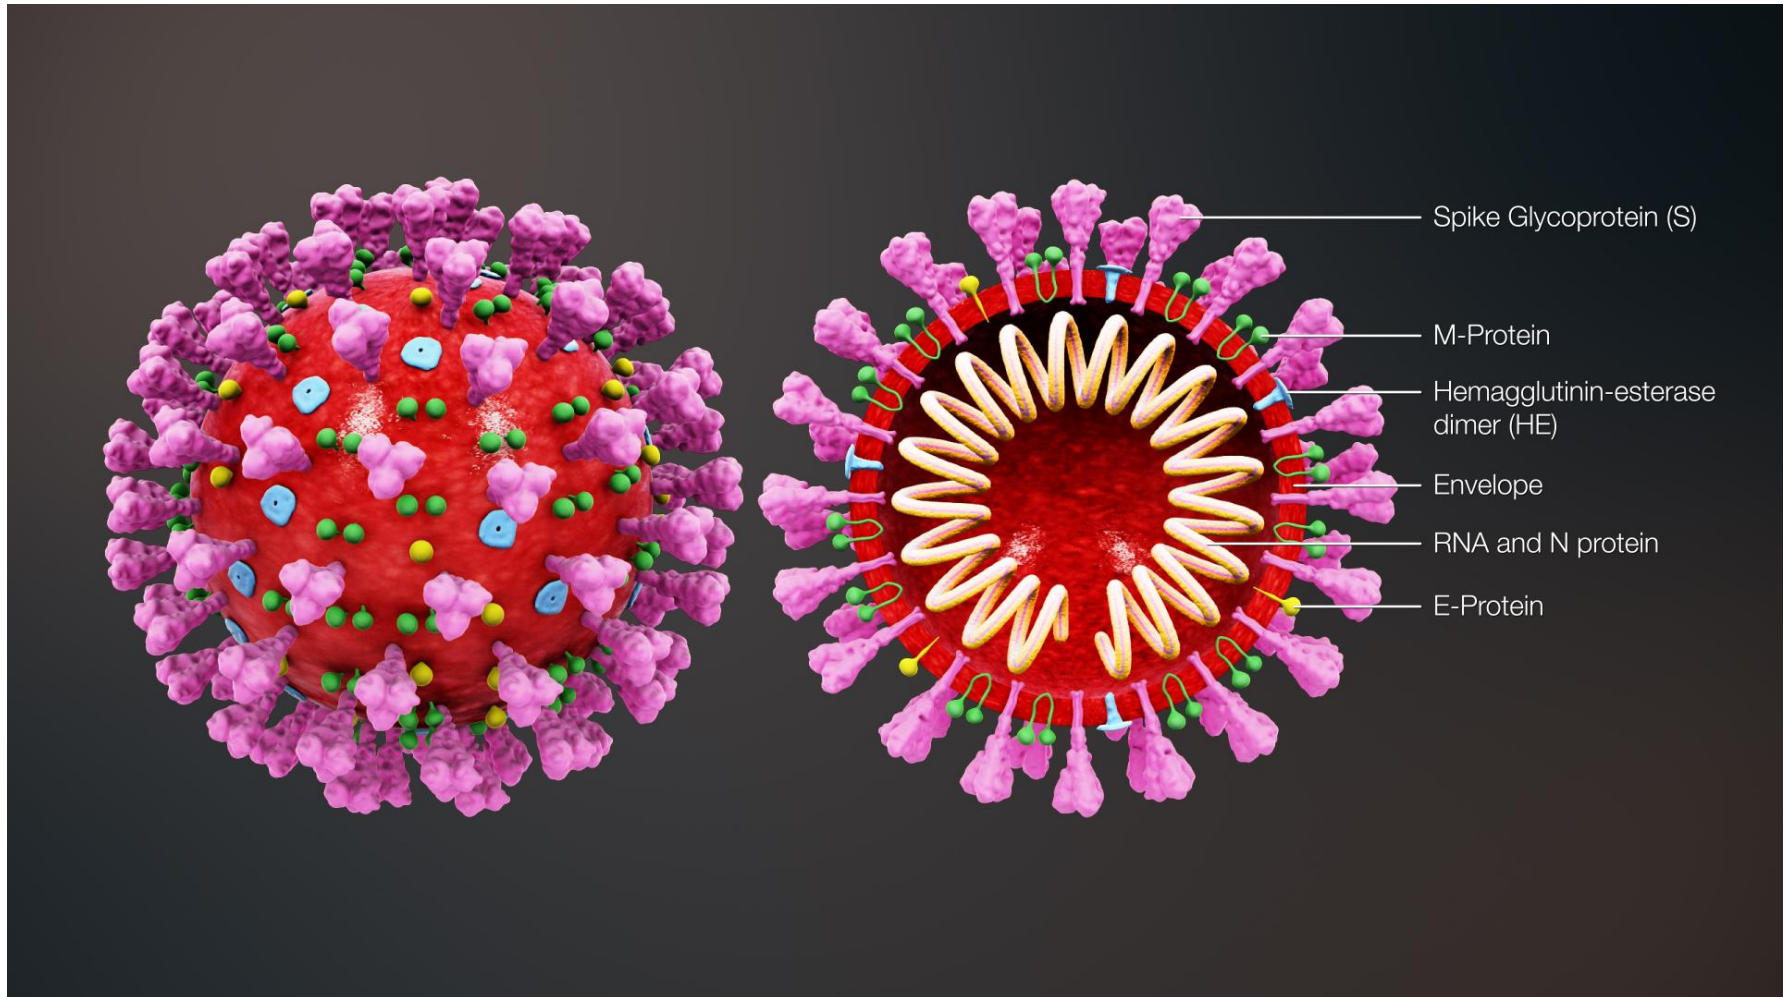



SARS-CoV-2: a beta-coronavirus with a genome in the form of a single RNA molecule of approx. 30,000 nt in length, and with (+) polarity

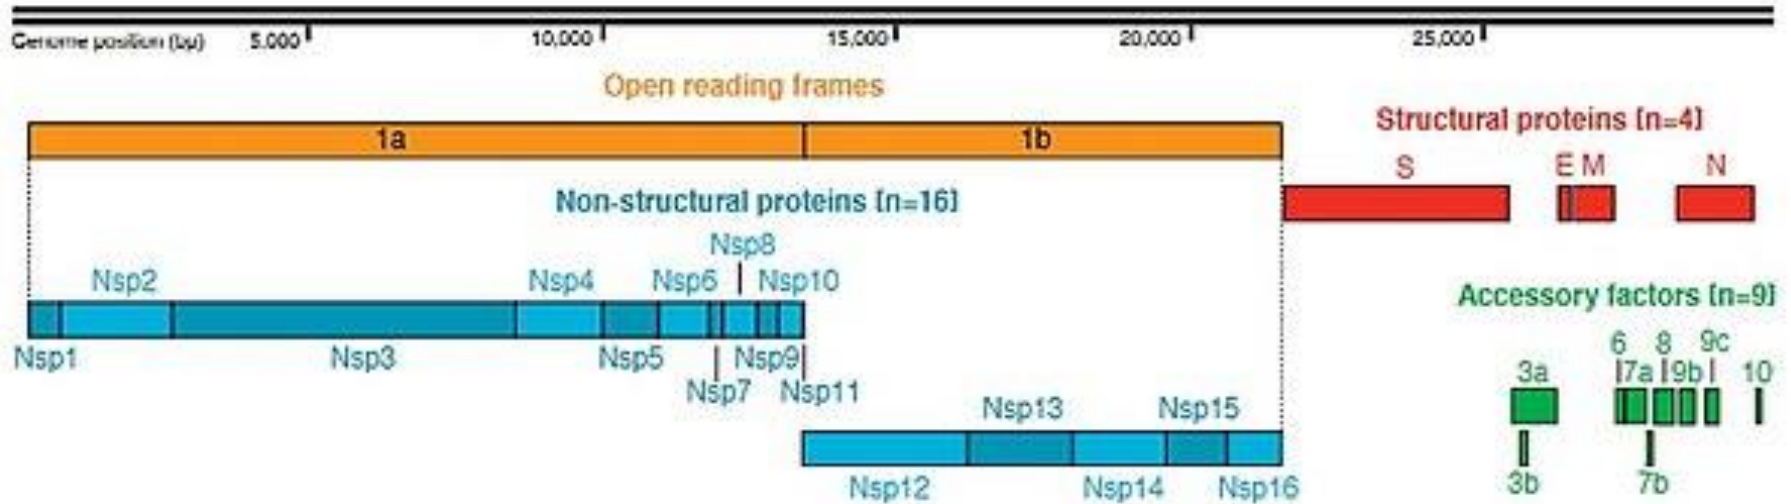


Wikipedia



SARS-CoV-2 replication cycle

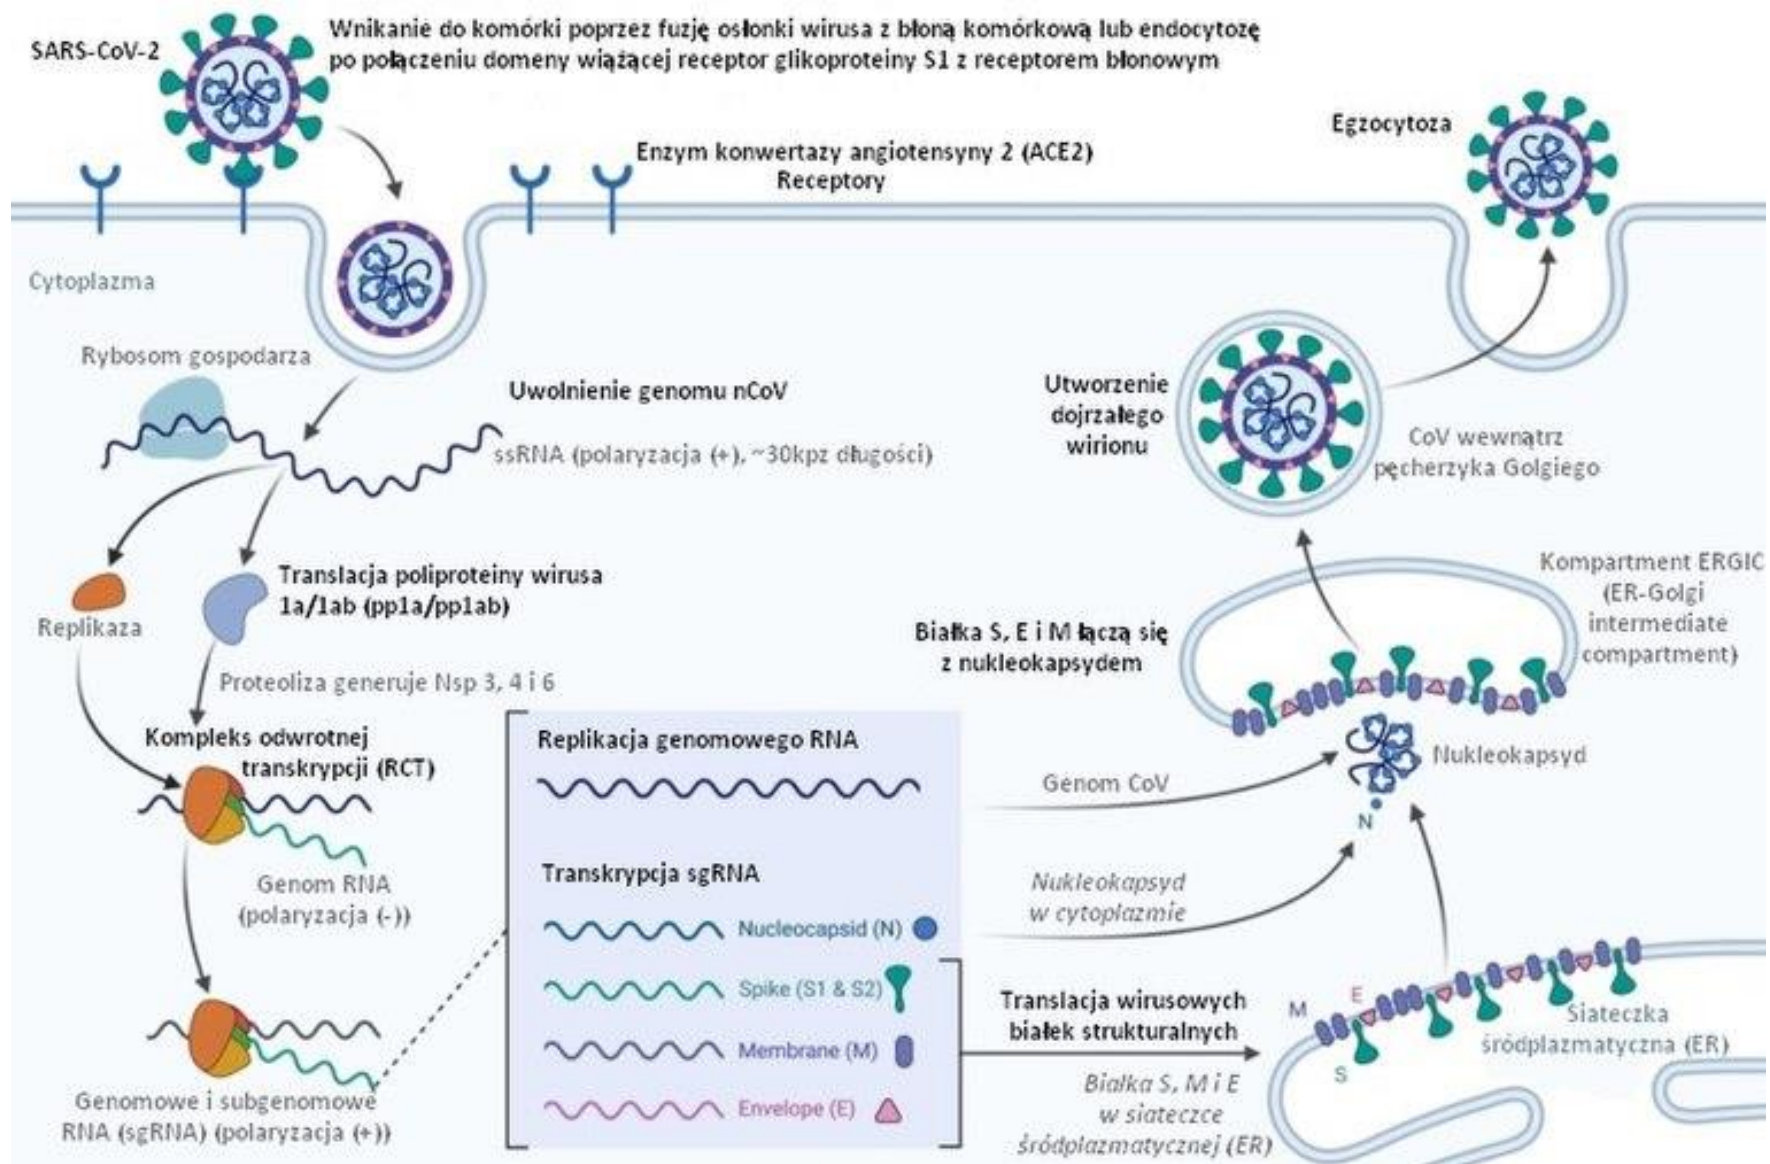

How can SARS-CoV-2 be detected?



Types of diagnostic tests used

Immunological tests

Detecting (using antibodies) anti-virus antibodies (does not necessarily detect the presence but the fact of passing infection): cassette, ELISA.




Detecting (using antibodies) the antigens of the virus (directly detecting its presence in the material)




Molecular tests


Detecting the genetic material of the virus (RNA) using RT-qPCR.



"Windows" of sensitivity of diagnostic tests

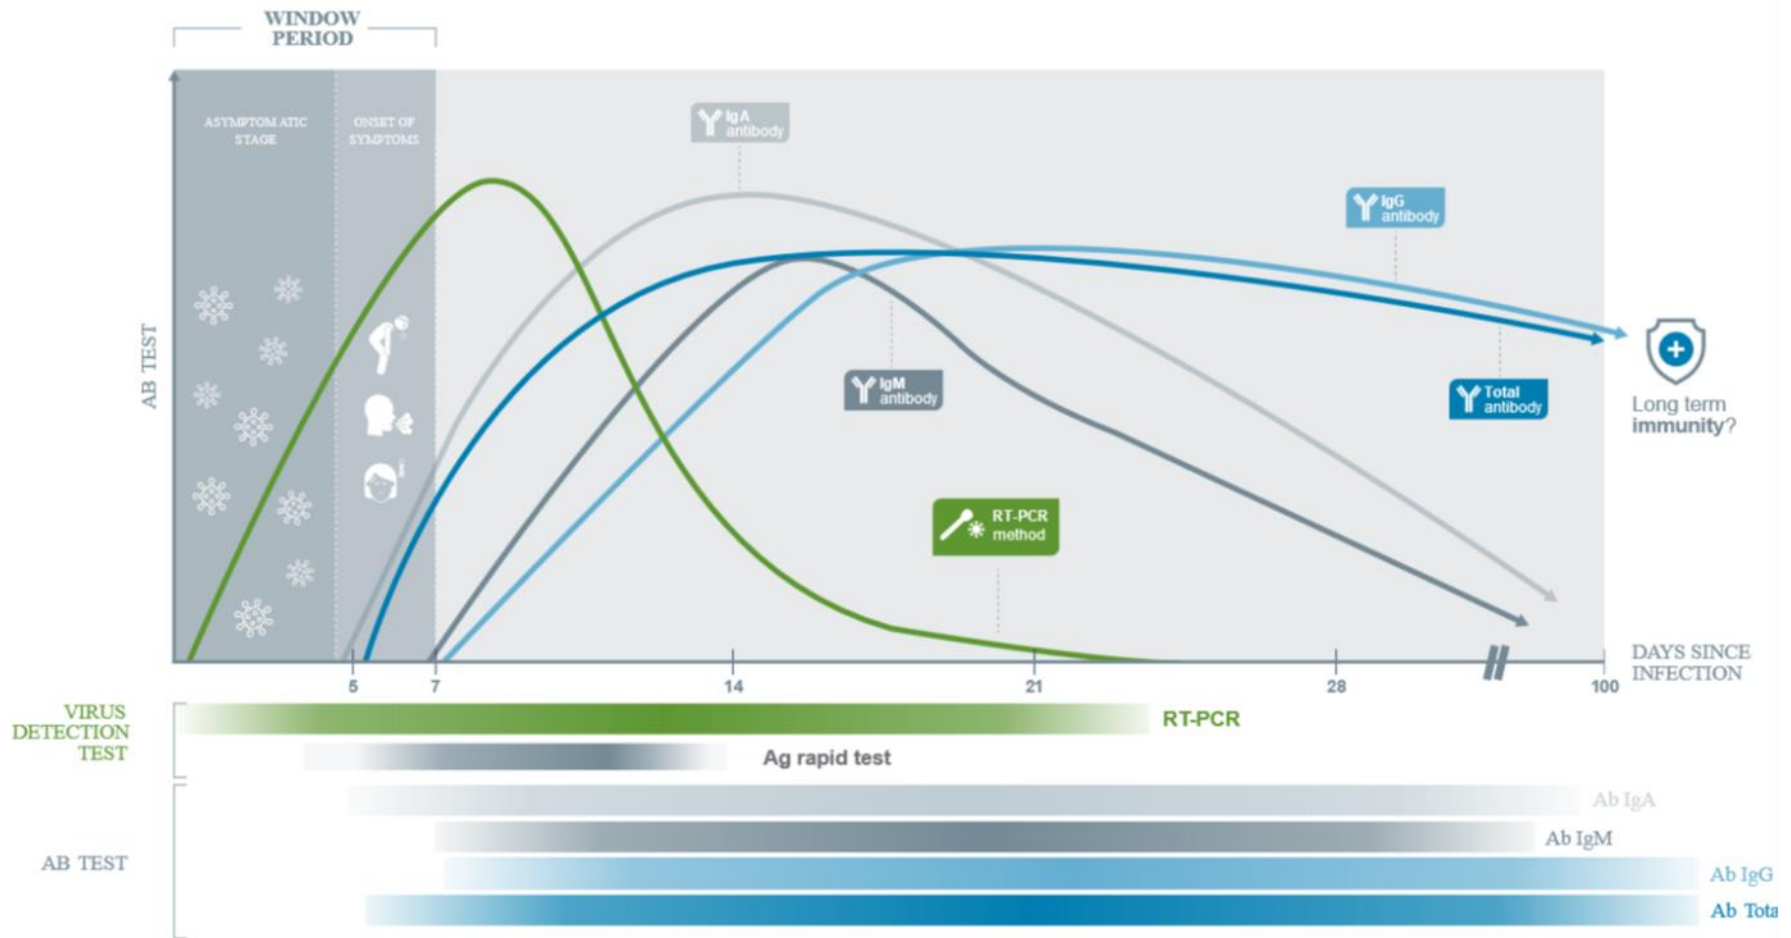

<https://www.synlab.com/news-publications/sars-cov-2/antigen-tests-for-sars-cov-2-detection>







How to isolate viral RNA?

First, the collection of material - preferably a **nasopharyngeal** swab.

Then lysis of the material: **enzymatic** (proteinase K digestion) or **chemical** (chaotropic salts such as GTC).

RNA recovery based on the affinity of nucleic acids for **silica resin** ("columns") or **ferromagnetic beads** ("beads").

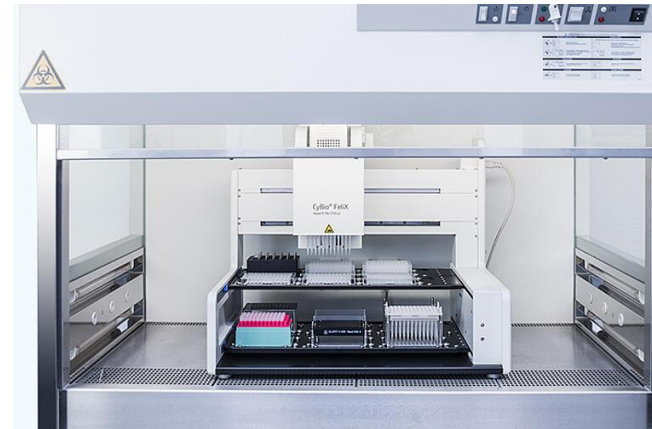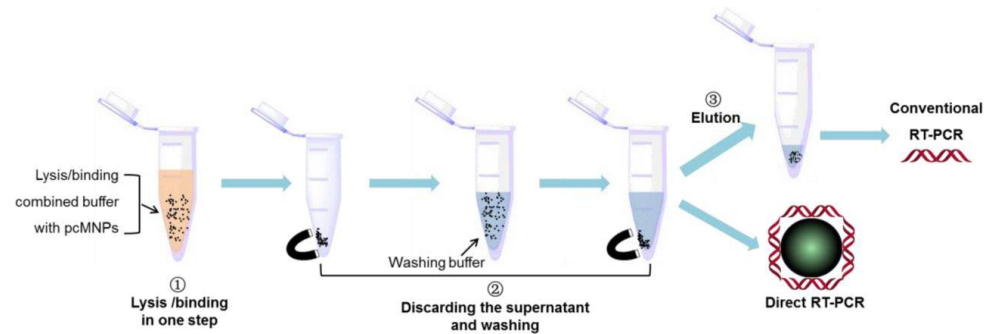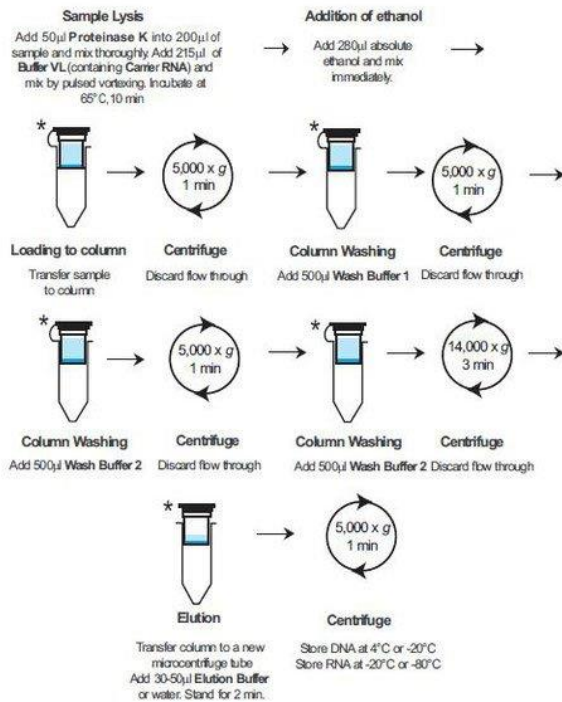

Open vs closed systems

Open systems

- Manual work (danger of contamination, not very efficient)
- open robots (you can choose different suppliers of plastics or reagents)






Closed systems

- high cost but better standardization
- "All-in-one" (isolation+RT-qPCR) or only isolation
- simplified operation
- „personal devices“
- problems with reagent availability
- Isolation + RTqPCR even in a few tens of minutes




TaqMan – hydrolysis probes



DNA Pol Exo !!!+

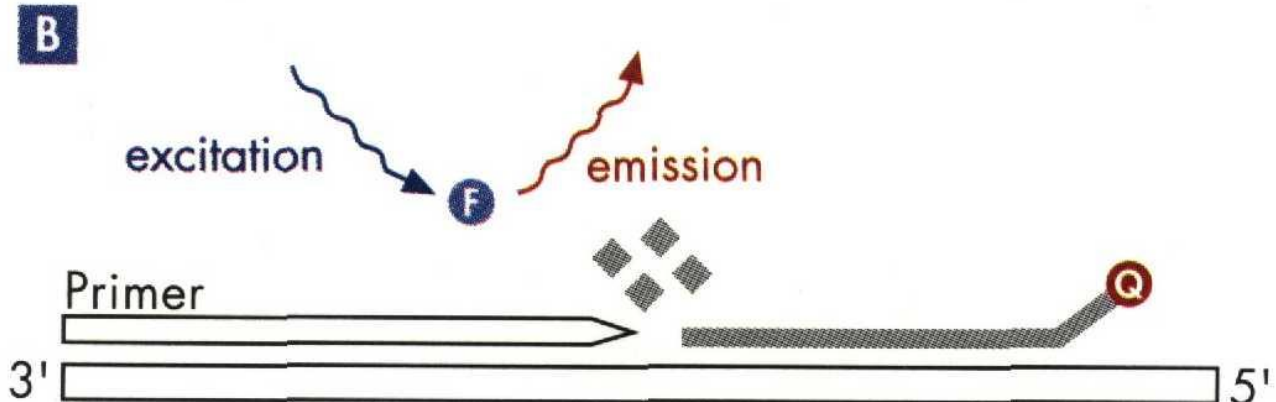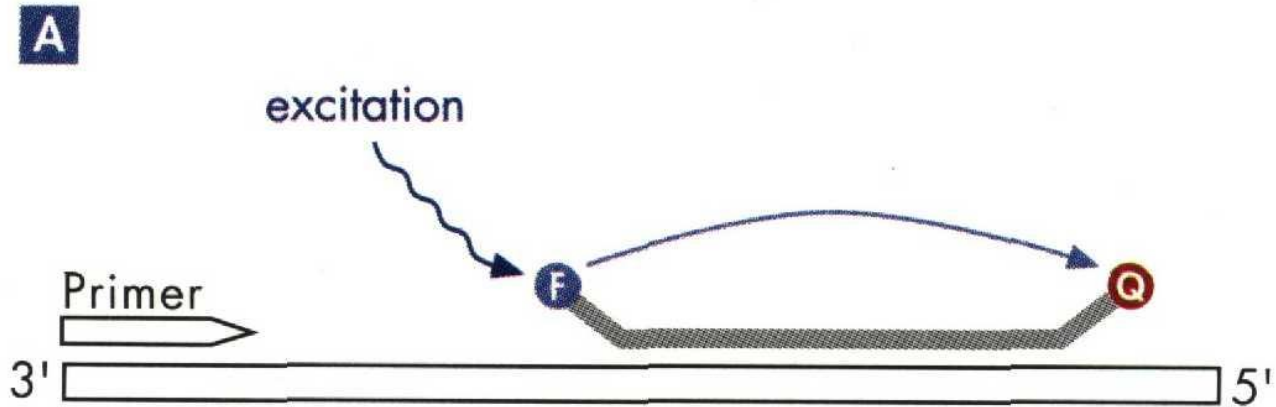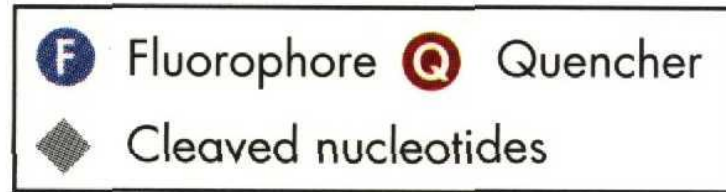

ABI, Roche (UPL)




Multiplex qPCR

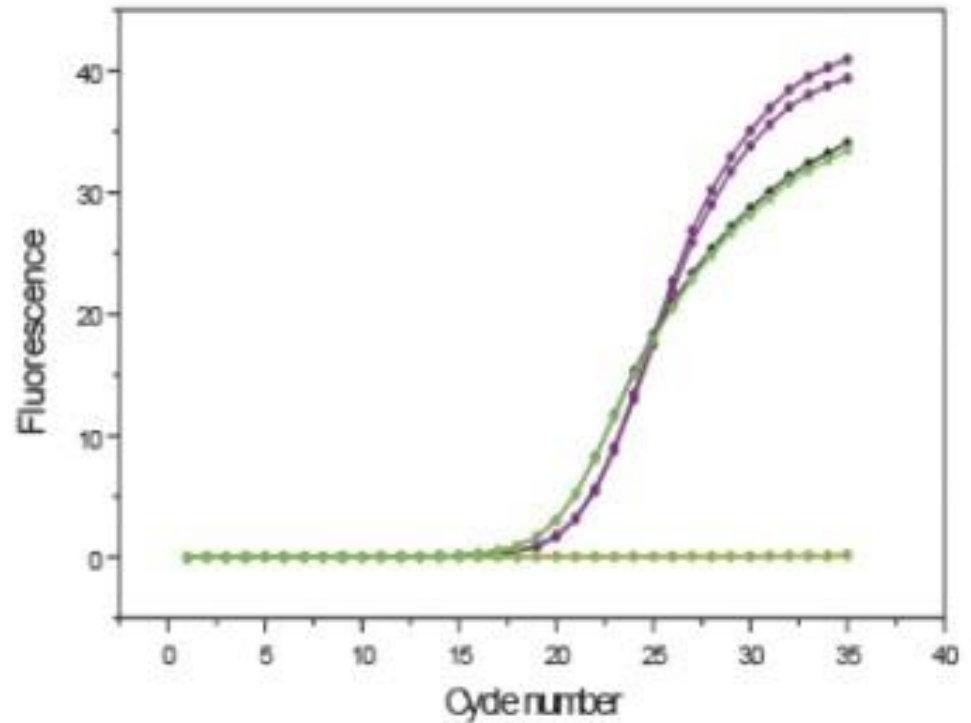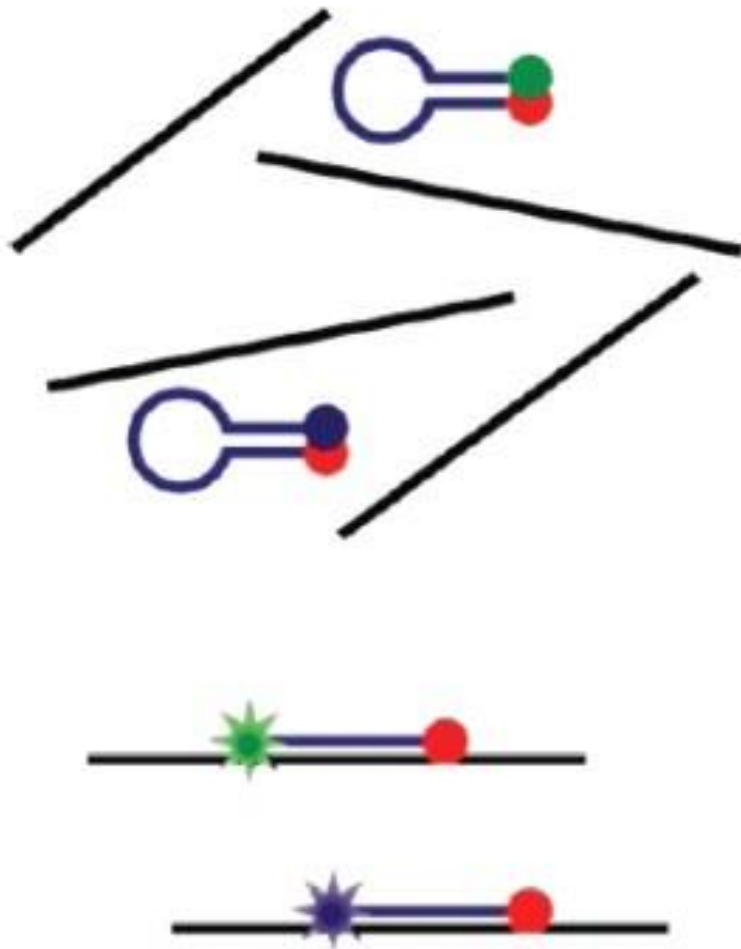

Different detection formats and different dyes allow detection of 2 or more products in a single reaction


(not possible with SYBR Green!!!)



What amplicons should be used in RT-qPCR ?

FIGURE 1

Relative positions of amplicon targets on the SARS coronavirus and the 2019 novel coronavirus genome

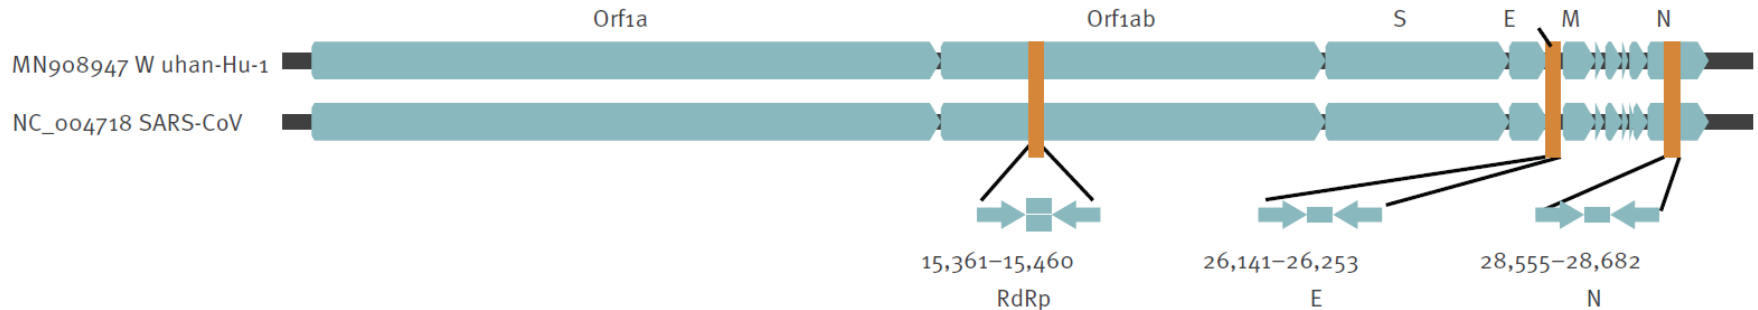


E: envelope protein gene; M: membrane protein gene; N: nucleocapsid protein gene; ORF: open reading frame; RdRp: RNA-dependent RNA polymerase gene; S: spike protein gene.

Numbers below amplicons are genome positions according to SARS-CoV, GenBank NC_004718.

Corman et al, Detection of 2019 novel coronavirus (2019-nCoV) by real-time RT-PCR. Euro Surveill. 2020 Jan;25(3)

In addition, control amplicons (not always all used at the same time):

- **SPIKE-IN RNA** (synthetic - isolation control only)
- **Internal control** (human mRNA - isolation and collection control!)




Sensitivity of the RT-qPCR method


FIGURE 3

Determination of limits of detection based on SARS coronavirus genomic RNA and 2019 novel coronavirus-specific in vitro transcribed RNA


A. E gene assay vs SARS-CoV: 5.2 c/r (95% CI: 3.7–9.6)

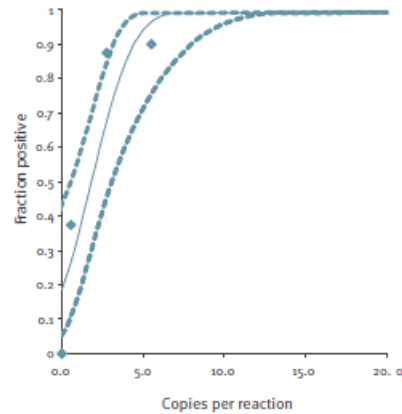


B. RdRp gene assay vs SARS-CoV: 3.8 c/r (95% CI: 2.7–7.6)

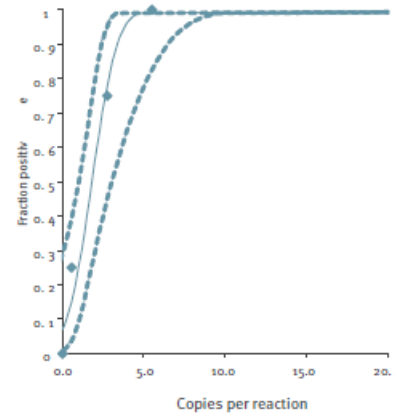

C. E gene assay vs 2019-nCoV IVT RNA: 3.9 c/r (95% CI: 2.8–9.8)

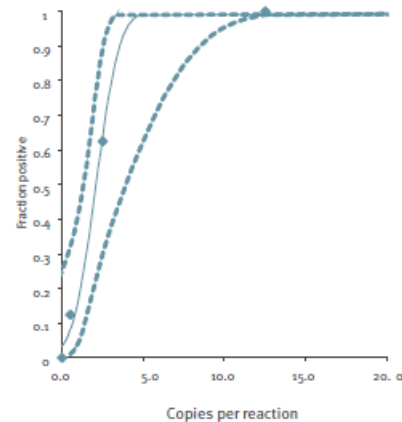


D. RdRp assay vs 2019-nCoV IVT RNA: 3.6 c/r (95% CI: 2.7–11.2)

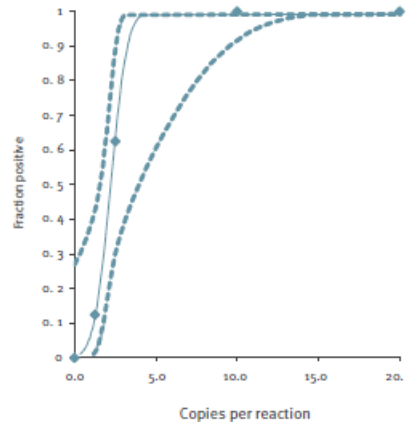


CI: confidence intervals; c/r: copies per reaction; IVT: in vitro-transcribed RNA.

Corman et al, Detection of 2019 novel coronavirus (2019-nCoV) by real-time RT-PCR. Euro Surveill. 2020 Jan;25(3)




Safety first!!!




Example result

Viral amplicons

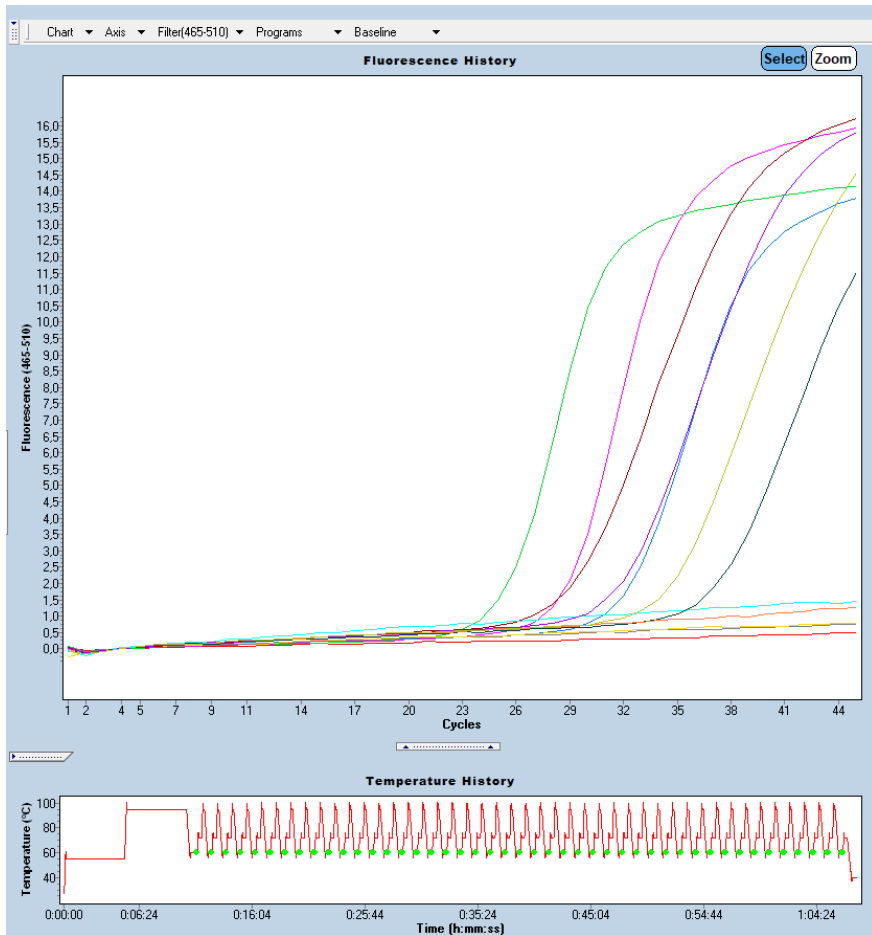

Control amplicons

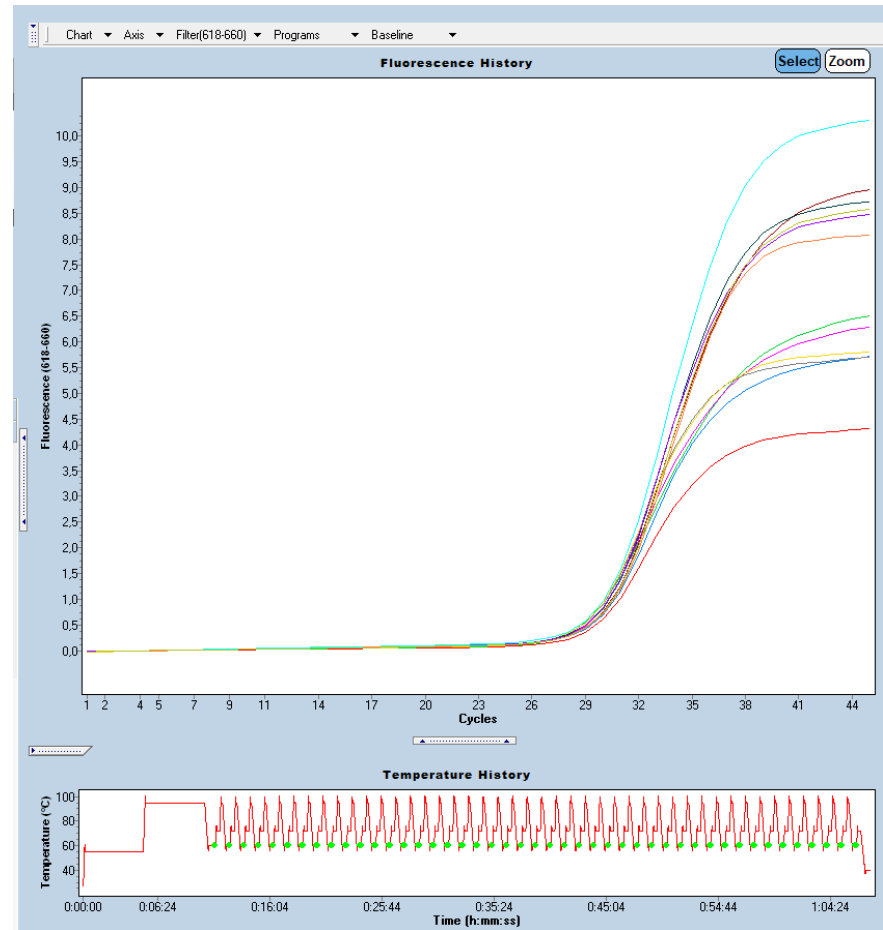

For more watch on YT: <https://www.youtube.com/watch?v=SNvGQJlcQfQ> (in polish)

